




SEMI - AUTOMATED PUMP STAND

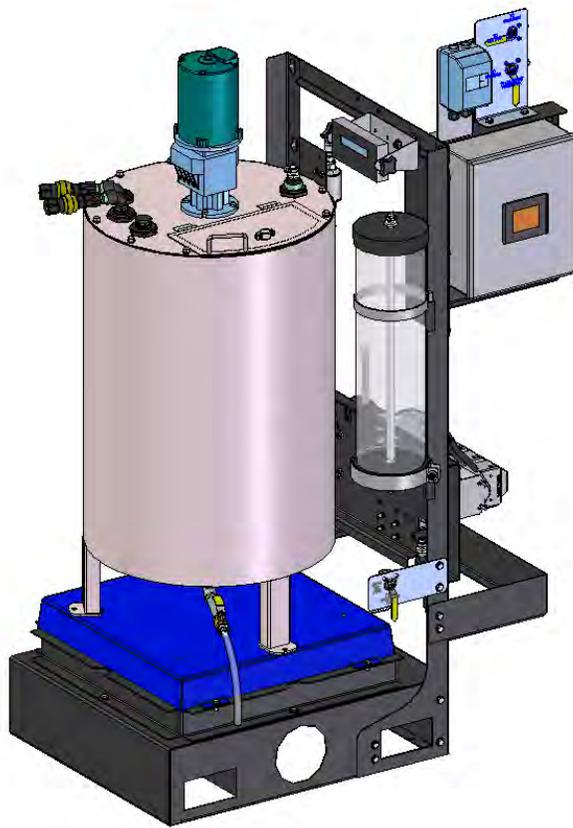

Operators Manual

Software Release: CPS v1.01



INTRODUCTION

Thank you for choosing USC, LLC for your equipment needs. We appreciate your business and will work diligently to ensure that you are satisfied with your choice.

OVERVIEW

The purpose of this manual is to provide you with the basic information needed to operate and maintain the Semi - Automated Pump Stand. It does not hold USC, LLC liable for any accidents or injuries that may occur.

OPERATOR RESPONSIBILITIES

As the purchaser/owner/operator of this equipment and control system, you have an obligation to install, operate, and maintain the equipment in a manner that minimizes the exposure of people in your care to any potential hazards inherent in using this equipment. It is critical that the owner of this equipment:

- Has a clear and documented understanding of the process this machine is being used in and of any resulting hazards or special requirements arising from this specific application.
- Allow only properly trained and instructed personnel to install, operate, or service this equipment.
- Maintain a comprehensive safety program involving all who work with this machine and other associated process equipment.
- Establish clear areas of staff responsibility (e.g. operation, setup, sanitation, maintenance, and repairs).
- Provide all personnel with necessary safety equipment.
- Periodically inspect the equipment to insure that the doors, covers, guards, and safety devices are in place and functioning, that all safety instructions and warning labels are intact and legible, and that the equipment is in good working order.
- In addition to the operating instructions, observe and enforce the applicable legal and other binding regulations, national and local codes.

As the person with the most to gain or lose from working safely, it is important that you work responsibly and stay alert. By following a few simple rules, you can prevent an accident that could injure or kill you or a co-worker.


SEMI - AUTOMATED PUMP STAND

- Do not operate, clean, or service this equipment until you have read and understood the contents of this manual. If you do not understand the information in this manual, bring it to the attention of your supervisor, or call your local USC dealer for assistance.
- Any operator who is known or suspected to be under the influence of alcohol or drugs should not be allowed to operate the equipment.
- Understand and follow the safety practices required by your employer and this manual.
- **PAY ATTENTION** to what you and other personnel are doing and how these activities may affect your safety.
- **Failure to follow these instructions may result in serious personal injury or death.**

RECEIVING YOUR EQUIPMENT

As soon as the equipment is received, it should be carefully inspected to make certain that it has sustained no damage during shipment and that all items listed on the packing list are accounted for. If there is any damage or shortages, the purchaser must immediately notify your USC dealer. Ownership passes to purchaser when the unit leaves the USC, LLC. premises. The purchaser is responsible for unloading and mounting all components of the equipment.

Document the serial number of the machine for future reference. The serial number is located on the upper left corner of the main panel mounting bracket.

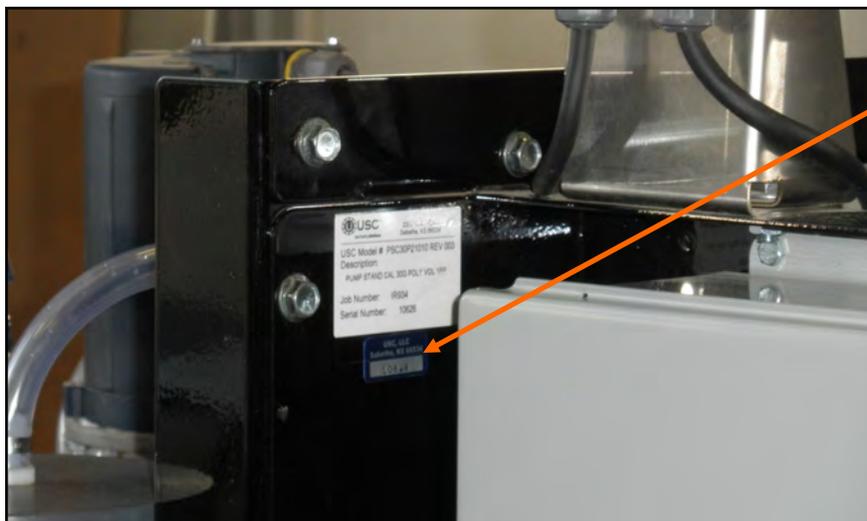

*Serial
Number*

SERIAL NUMBER: _____

TABLE OF CONTENTS

<u>Section</u>	<u>Contents</u>	<u>Page #</u>
Section A	Safety Instructions.....	5
Section B	Installation	12
Section C	Mechanical Operation.....	14
	Semi - Automated Pump Stand Overview	14
	Mix Tank and Calibration Tube	16
	Peristaltic Pump Heads and Motor	17
	Flow Meter and Pump Stand Valves	18
Section D	Electrical Operation	20
	Start Up Screen	21
	Main Screen	22
	Settings Screen.....	24
	Configuration Screen	25
	Select Chemical and Edit Chemical Screens.....	26
	Calculator Screen.....	27
Section E	Calibration	28
	Pump Calibration	28
	Flow Meter Calibration	29
Section F	Troubleshooting.....	30
Section G	Maintenance	31
Section H	Storage.....	32
Section I	Mechanical Drawings	34
Section J	Limited Warranty.....	61

SAFETY INSTRUCTIONS

SECTION A

Every year accidents in the work place maim, kill, and injure people. Although it may be impossible to prevent all accidents, with the right combination of training, operating practices, safety devices, and operator vigilance, the number of accidents can be significantly reduced. The purpose of this section is to educate equipment users about hazards, unsafe practices, and recommended hazard avoidance techniques.

SAFETY WORDS AND SYMBOLS

It is very important that operators and maintenance personnel understand the words and symbols that are used to communicate safety information. Safety words, their meaning and format, have been standardized for U.S. manufacturers and published by the American National Standards Institute (ANSI). The European Community (E.C.) has adopted a different format based on the International Standards Organization (I.S.O.) and applicable machinery directives. Both formats are presented below. Graphic symbols are not standardized, but most manufacturers will use some variation of the ones seen in this manual.



Indicates an imminently hazardous situation which, if not avoided, **will** result in death or serious injury.



Indicates a potentially hazardous situation which, if not avoided, **could** result in death or serious injury.



Indicates a potentially hazardous situation which, if not avoided, **may** result in minor or moderate injury and/or property damage.



Provides additional information that the operator needs to be aware of to avoid a potentially hazardous situation.



Mandatory Lockout Power Symbol. Disconnect, lockout, and tagout electrical and other energy sources before inspecting, cleaning, or performing maintenance on this panel.



International Safety Alert Symbol. The exclamation point (!) surrounded by a yellow triangle indicates that an injury hazard exists. However, it does not indicate the seriousness of potential injury. The exclamation point (!) is also used with the DANGER, WARNING, and CAUTION symbols so the potential injury is indicated.



Electrocution Hazard Symbol. This symbol indicates that an electrocution hazard exists. Serious injury or death could result from contacting high voltage.



International Electrocution Hazard. This symbol indicates that an electrocution hazard exists. Serious injury or death could result from contacting high voltage.



Mandatory Read Manual Action Symbol. (I.S.O. format) This symbol instructs personnel to read the Operators Manual before servicing or operating the equipment.



Mandatory Read Manual Action Symbol. This symbol instructs personnel to read the Operators Manual before servicing or operating the equipment.

NOTICE

Notice is used to notify people of important installation, operation, or maintenance information which is not hazard related.

LOCKOUT / TAGOUT PROCEDURES

Lockout/Tagout is the placement of a lock/tag on an energy isolating device in accordance with an established procedure. When taking equipment out of service to perform maintenance or repair work, always follow the lockout/tagout procedures as outlined in ANSI Z344.1 and/or OSHA Standard 1910.147. This standard “requires employers to establish a program and utilize procedures for affixing appropriate lockout devices or tagout devices to energy isolating devices and to otherwise disable machines or equipment to prevent unexpected energizing, start-up, or release of stored energy in order to prevent injury to employees.”

HAZARD REVIEW

Electrocution Hazard



Electrocution accidents are most likely to occur during maintenance of the electrical system or when working on or near exposed high voltage wiring. This hazard does not exist when the electrical power has been disconnected, properly locked, and tagged out.

Automatic Start Hazard



This Semi - Automated Pump Stand may be controlled by an automated system and may start without warning. Failure to properly disconnect, lockout, and tagout all energy sources of remotely controlled equipment creates a very hazardous situation and could cause injury or even death. PLEASE STAY CLEAR AND BE ALERT.

SEMI - AUTOMATED PUMP STAND

YOU are responsible for the **SAFE** operation and maintenance of your USC, LLC pump stand. **YOU** must ensure that you and anyone else who is going to operate, maintain, or work around the pump stand be familiar with the operating and maintenance procedures and related **SAFETY** information contained in this manual. This manual will take you step-by-step through your working day and alert you to good safety practices that should be adhered to while operating the pump stand.

Remember, **YOU** are the key to safety. Good safety practices not only protect you, but also the people around you. Make these practices a working part of your safety program. Be certain that **EVERYONE** operating this equipment is familiar with the recommended operating and maintenance procedures and follows all the safety precautions. Most accidents can be prevented. Do not risk injury or death by ignoring good safety practices.

- Semi - Automated Pump Stand owners must give operating instructions to operators or employees before allowing them to operate the machine, and at least annually thereafter per OSHA (Occupational Safety and Health Administration) regulation 1928.57.
- The most important safety device on this equipment is a **SAFE** operator. It is the operator's responsibility to read and understand **ALL** Safety and Operating instructions in the manual and to follow them. All accidents can be avoided.
- A person who has not read and understood all operating and safety instructions is not qualified to operate the machine. An untrained operator exposes himself and bystanders to possible serious injury or death.
- Do not modify the equipment in any way. Unauthorized modification may impair the function and/or safety and could affect the life of the equipment.
- Think **SAFETY!** Work **SAFELY!**


GENERAL SAFETY

1. Read and understand the Operator's Manual and all safety signs before operating, maintaining, adjusting or unplugging the Calibratable Pump Stand.
2. Only trained persons shall operate the seed treater. An untrained operator is not qualified to operate the machine.
3. Have a first-aid kit available for use should the need arise, and know how to use it.



SEMI - AUTOMATED PUMP STAND

4. Provide a fire extinguisher for use in case of an accident. Store in a highly visible place.
5. Do not allow children, spectators or bystanders within hazard area of machine.
6. Wear appropriate protective gear. This includes but is not limited to:
 - A hard hat
 - Protective shoes with slip resistant soles
 - Protective goggles
 - Heavy gloves
 - Hearing protection
 - Respirator or filter mask
7. Place all controls in neutral or off, stop motor, and wait for all moving parts to stop. Then disable power source before servicing, adjusting, repairing, or unplugging.
8. Review safety related items annually with all personnel who will be operating or maintaining the Semi - Automated Pump Stand.



OPERATING SAFETY:

1. Read and understand the Operator's Manual and all safety signs before using.
2. Disconnect and disable electrical supply completely and wait for all moving parts to stop before servicing, adjusting, repairing or unplugging.
3. Clear the area of bystanders, especially children, before starting.
4. Be familiar with the machine hazard area. If anyone enters hazard area, shut down machine immediately. Clear the area before restarting.
5. Keep hands, feet, hair and clothing away from all moving and/or rotating parts.
6. Stay away from overhead obstructions and power lines during operation and transporting. Electrocution can occur without direct contact.
7. Do not operate machine when any guards are removed.
8. Inspect welds and repair if needed.

PLACEMENT SAFETY

1. Move only with the appropriate equipment
2. Stay away from overhead power lines when moving pump stand. Electrocutation can occur without direct contact.
3. Be familiar with machine hazard area. If anyone enters hazard areas, shut down machine immediately. Clear the area before restarting.
4. Operate the pump stand on level ground free of debris. Anchor the pump stand to prevent tipping or upending.



Before placement of the pump stand, be sure that ground is reasonably level. The pump stand may topple or work improperly if the ground is too uneven, damaging the equipment and/or causing personal injury.

MAINTENANCE SAFETY

1. Review the Operator's Manual and all safety items before working with, maintaining or operating the pump stand.
2. Place all controls in neutral or off, stop motors, disable power source, and wait for all moving parts to stop before servicing, adjusting, repairing or unplugging.
3. Follow good shop practices:
Keep service area clean and dry.
Be sure electrical outlets and tools are properly grounded.
Use adequate light for the job at hand.
4. Keep hands, feet, hair and clothing away from all moving and/or rotating parts.
5. Clear the area of bystanders, especially children, when carrying out any maintenance and repairs or making any adjustments.
6. Before resuming work, install and secure all guards when maintenance work is completed.
7. Keep safety signs clean. Replace any sign that is damaged or not clearly visible.



SAFETY SIGNS

1. Keep safety signs clean and legible at all times.
2. Replace safety signs that are missing or have become illegible.
3. Replaced parts that displayed a safety sign should also display the current sign.
4. Safety signs are available from your Authorized Dealer.

How to Install Safety Signs:

- Be sure that the installation area is clean and dry.
- Be sure temperature is above 50°F (10°C).
- Decide on the exact position before you remove the backing paper.
- Remove the smallest portion of the split backing paper.
- Align the sign over the specified area and carefully press the small portion with the exposed sticky backing in place.
- Slowly peel back the remaining paper and carefully smooth the remaining portion of the sign in place.
- Small air pockets can be pierced with a pin and smoothed out using the piece of sign backing paper.



Located on the USC equipment you will find safety labels. Always be sure to read and follow all directions on the labels.



Guards provided with USC Semi - Automated Pump Stand are to remain in place during operation.

**SECTION
B**

INSTALLATION



HIGH VOLTAGE ~ Always disconnect the power source before working on or near the control panel or lead wires.



HIGH VOLTAGE ~ Use insulated tools when making adjustments while the controls are under power.



Permanent installation may require additional electrical cords, chemical tubing, and air lines, since each installation is unique.

SET-UP

The following steps outline the initial set-up of your USC Semi - Automated Pump Stand :

1. Clear the area of bystanders, especially small children, before moving.
2. Be sure there is enough clearance from overhead obstructions and power lines or other equipment to move the machine into its working position.
3. Using a forklift, place the pump stand in the desired position on a level surface.



USC highly recommends that the pump stand be set up inside a building or any covered structure to protect the machine from weathering.

4. Inspect pump stand thoroughly for screws, bolts, fittings, etc. which may have come loose during shipping.
5. The pump stand(s) should be placed on level ground close to the seed treater.

SEMI - AUTOMATED PUMP STAND

6. The Semi - Automated Pump Stand is equipped with a 110 volt plug in cord for both the mix motor and the panel it plugs into. A standard wall socket is adequate as long as it is 4 amps or greater on the breaker.



7. For LPX, LX and MX treaters, attach the chemical tubing from the pump stand(s) to the atomizer plumbing on the seed treater (left). For all other treaters additional tubing can be added or removed to accommodate your set-up.



8. For pump stands operating in the "AUTO" mode, a yellow two wire cable connection is required from the auxiliary port on the pump stand control box to the treater control panel.




USC highly recommends that the Pump Stand be set up inside a building or any covered structure to protect the machine from weathering.


SECTION
C

MECHANICAL OPERATION

SEMI - AUTOMATED PUMP STAND OVERVIEW

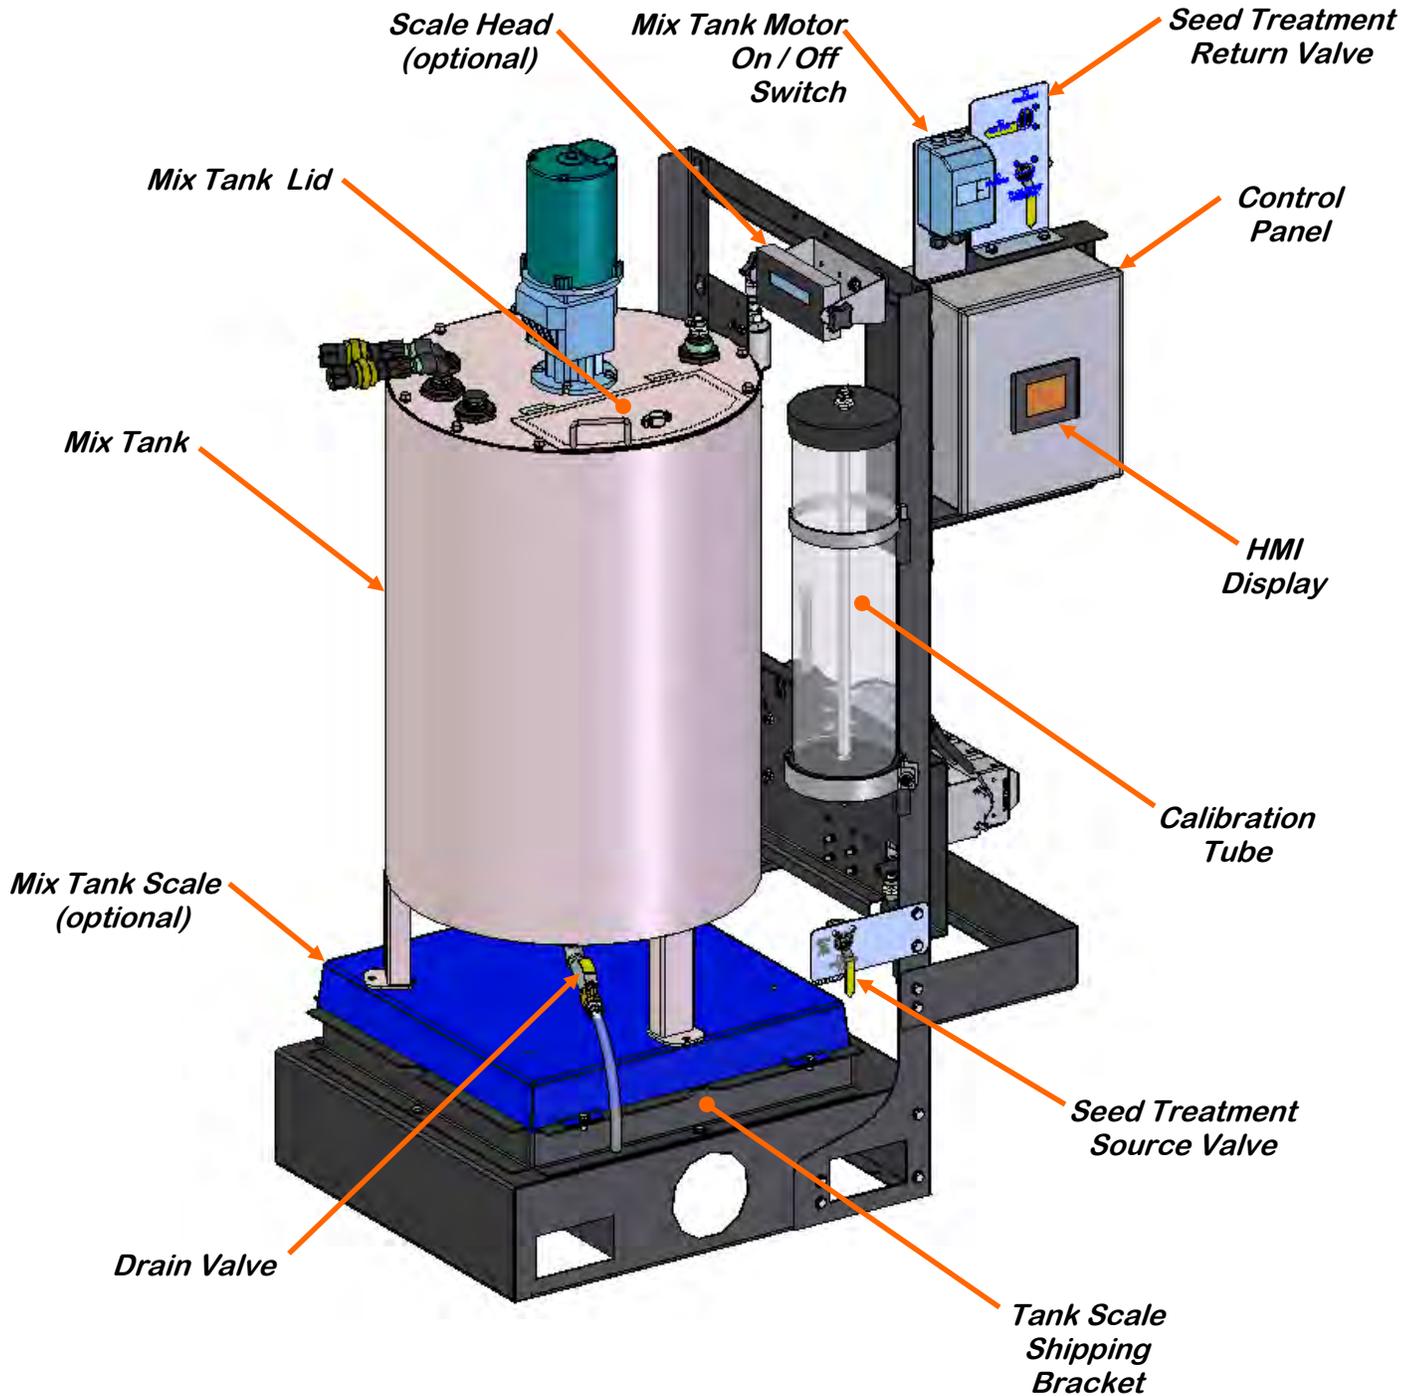

SEMI - AUTOMATED PUMP STAND OVERVIEW

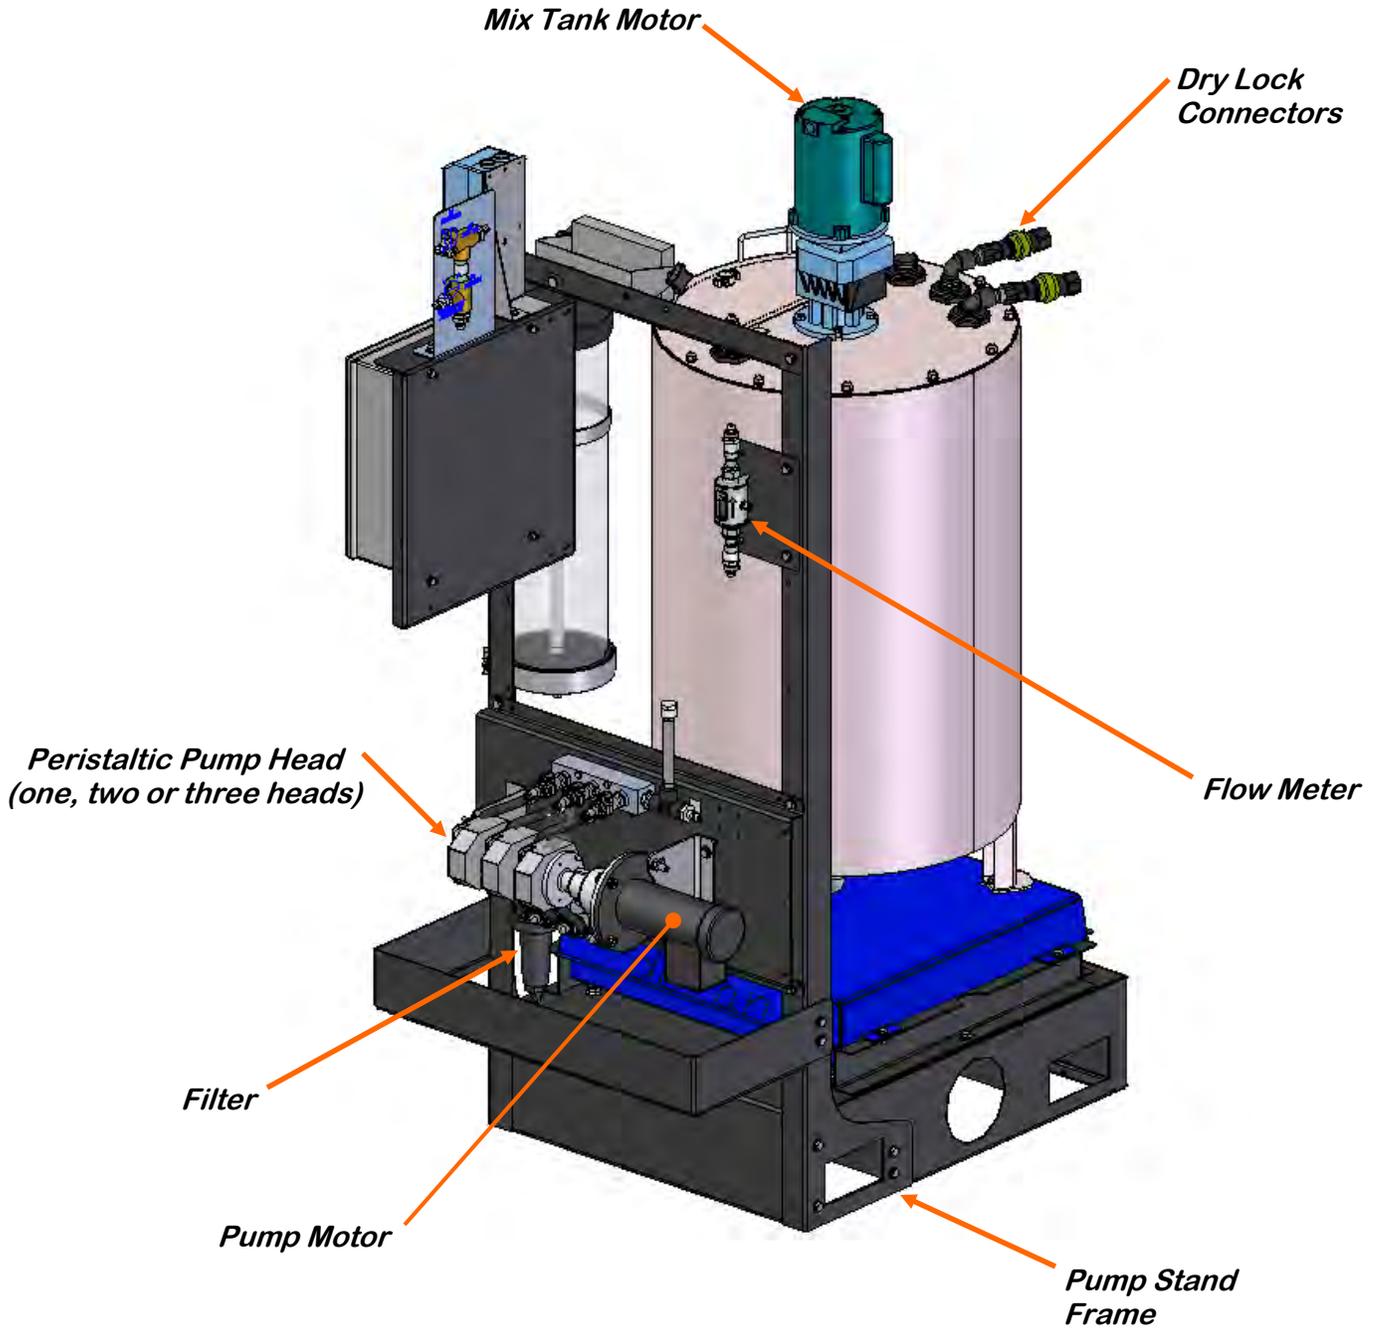

SEMI - AUTOMATED PUMP STAND


MIX TANK

The USC Semi - Automated Pump Stand is equipped with a fully modular, touch screen to control the pump stand. This pump stand will include a 30 or 60 gallon chemical mix tank that is either of stainless steel or poly construction. This chemical mix tank will have electric drive agitation that is turned on or off at the pump stand with a manual switch. The agitator should be running at all times when treatment is present in the mix tank to keep the chemical mixed and in a suspended state. The tank is equipped with a shut-off, drain plug, and drain valve located on the bottom. The top of the tank also includes 3 extra ports which the operator can use to direct fill into the tank (see below).



CALIBRATION TUBE



The Semi - Automated Pump Stand is equipped with a calibration tube which is used to check the liquid flow rate. The calibration tube measures in ounces, on a 0-340 scale and millimeters on a 0-10000 scale. Manual valves direct liquid from different areas to keep all liquid contained. This creates a closed chemical system so that the operator can manually check the calibration of the chemical flow rate without handling any of the chemical.

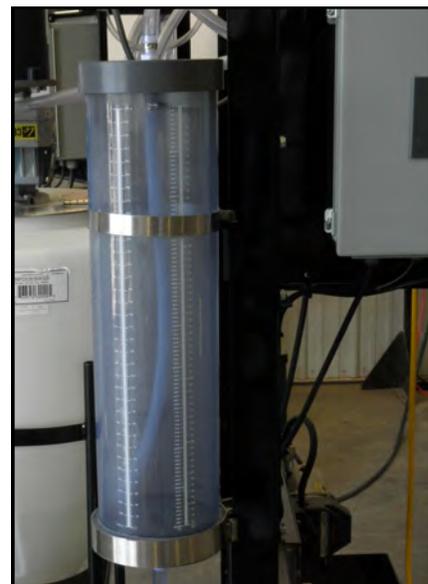


PERISTALTIC PUMP HEADS AND MOTOR

The Semi - Automated Pump Stand utilizes a variable speed pump motor and special noprrene pump tubing for liquid metering. The pump comes equipped with either 1, 2 or 3 peristaltic pump heads. Liquid will only come into contact with the inside diameter of the pump tubing and not the pump. This allows for easy cleanup and less maintenance of the pump.

To open the pump head, lift the lever upward. Place the pump tubing inside the pump head so it fits inside the notches and above the rollers. Lower the lever back down to close the pump head, clamping the hose inside the head. Wear or fatiguing of the tubing within the pump head due to compression is normal. When tubing becomes worn or chemical rates begin to slow down, open the pump head and move the tubing to a different position. If the entire piece of tubing becomes worn, simply replace with a new section. When not using the pump stand for several days or when storing, open the pump head and remove the tubing to prevent any extra compression.

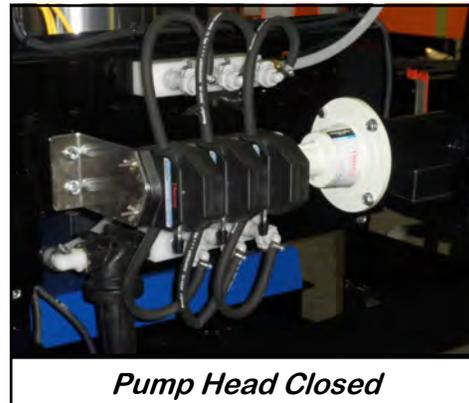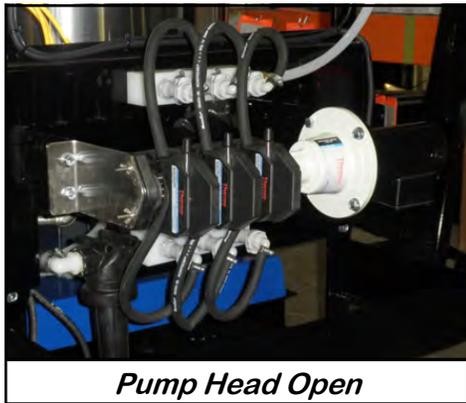

If a very low rate is needed, a section of tubing can be removed to force the pump motor to run at a higher speed. This allows for a more consistent flow rate. When removing the tubing, uncouple it from the manifold (below, right). If the tubing is unclamped from the pump head but left coupled in the manifold (below, left), the pump will suck air and cause flow rates to be very inconsistent.

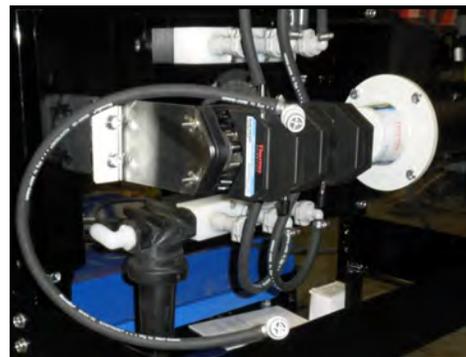

SEMI - AUTOMATED PUMP STAND

FLOW METER

Each Semi - Automated Pump Stand comes with either a volumetric or mass flow meter. A flow meter is used to perform real-time chemical flow adjustments and monitoring without the operator having to handle the chemical. The flow meter reading will be displayed on the HMI touch screen and can be set to read in oz/min or ml/min.



Volumetric Flow Meter



Mass Flow Meter

PUMP STAND VALVES

Seed Treatment Source Valve: This valve controls where the pump is drawing liquid from. It allows liquid to be pulled from either the bottom of the mix tank or the calibration tube.




Drawing chemical from the bottom of the Mix Tank



Drawing chemical from the bottom of the Calibration Tube

SEMI - AUTOMATED PUMP STAND

Seed Treatment and Return Valves: The bottom valve directs the liquid to the top valve or to the seed treater. The top valve directs the liquid coming from the mix tank or calibration tube or back to the calibration tube or mix tank for re-circulation.

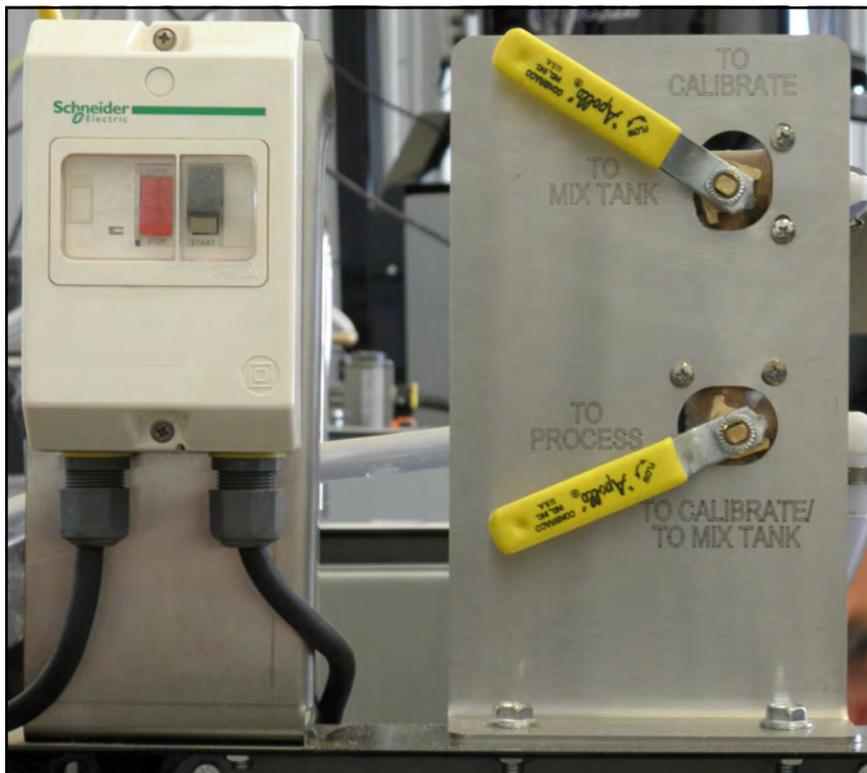

Proper calibration of the liquid system is critical to achieve a proper granular/chemical mixture. Use the calibration procedure on page 28 and 29 to determine liquid flow rate.

Emptying the remaining liquid can be done by using the reverse function on the control panel. This will pump liquid back into the mix tank. Then drain the remaining liquid into a suitable container. Clean water should be pumped through the calibration tube and mix tank when finished.



Always dispose of chemical or diluted chemical according to your local, state, and federal regulations.



Only you, the operator, can determine the length of time required to completely rinse all chemical residue from the tank and plumbing system.

SECTION
D

ELECTRICAL OPERATION



HIGH VOLTAGE ~ Always disconnect the power source before working on or near the control panel or lead wires.



HIGH VOLTAGE ~ Use insulated tools when making adjustments while the controls are under power.



AUTHORIZED PERSONNEL only shall work on the control panel. Never allow anyone who has not read and familiarized themselves with the owner's manual to open or work on the control panel. e switch is turned on,

This section provides a general overview and description of the operator controls for the Semi - Automated Pump Stand.

General Panel Descriptions

- The Semi - Automated Pump Stand Panel is a plug connected enclosure that is located on each pump stand frame. This panel connects the pump stand electrical components to the Treater Control Panel.

SEMI - AUTOMATED PUMP STAND

SEMI - AUTOMATED PUMP STAND CONTROL PANEL

The following pages explain the function of the touch screen controls.


USC START UP SCREEN

While the system is booting up, the pump stand touch screen will display a timer bar at the bottom of the Start Up Screen. Once the timer bar reaches the end it will advance the user to the Main Screen.



MAIN SCREEN

This screen informs the operator which chemical is currently selected, ounces of the chemical being applied per minute and total ounces used. It can also be displayed in metric (see page 25). The buttons on the left side and bottom of the screen allows for control / adjustment of system operations.

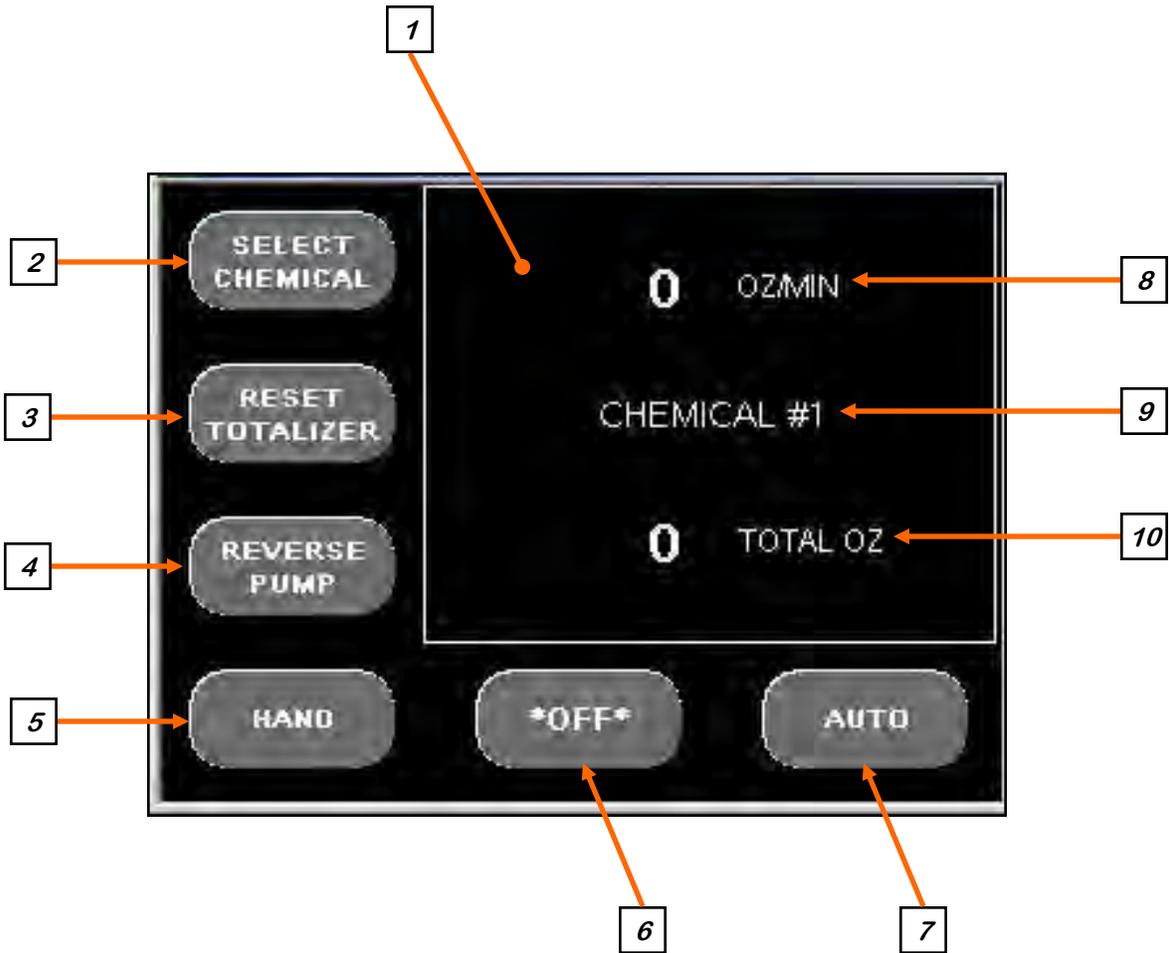

Main Screen Button Descriptions

1. "CHEMICAL STATUS BOX": Displays the chemical currently selected, flow rate in ounces per minute and total ounces used. The entire box is also a button. When pushed it advances the operator to the Settings screen.

2. "SELECT CHEMICAL" BUTTON: Advances the operator to the Select Chemical Screen.

3. "RESET TOTALIZER" BUTTON: Resets the totalizer to zero.

4. "REVERSE PUMP" BUTTON: Reverses the pump motor.

NOTICE Anytime the pump is run in reverse or after the Atomizer is primed the operator must reset the totalizer on the screen before start up. This step is necessary to insure the totalizers accuracy for the run.

5. "HAND" BUTTON: Turns the pump motor ON and OFF. When this button is active the text increases in size and there is an asterisk before and after the text.

6. "OFF" BUTTON: Turns the pump motor off. When this button is active the text increases in size and there is an asterisk before and after the text.

7. "AUTO" BUTTON: This button is used when the pump stand is attached to an auxiliary contact on the treater. This allows the treater to turn the pump on and off at the appropriate time. When this button is active the text increases in size and there is an asterisk before and after the text.

8. "OUNCES PER MINUTE": Displays the ounces of chemical per minute being applied. It also may be displayed in milliliters.

9. "CHEMICAL NAME": Displays the name of the chemical that is selected.

10. "TOTAL OUNCES": Displays in real time the amount of chemical that has been applied.

SETTINGS SCREEN


1. "TARGET RATE": When this button is pushed a keypad (bottom) will appear on the screen. This allows the operator to set an application target rate in ounces or milliliters per minute.

2. SCREEN EXIT: This button is used to exit back to the previous screen. It's functionality is the same throughout the HMI display.

3. APPLICATION METHOD: Pressing one of these two buttons determines what method the operator will use for an application rate. Ounces per minute or pump speed .

4. "PUMP PERCENTAGE RATE": When this button is pushed a keypad (bottom) will appear on the screen. This allows the operator to set an application target rate based on pump speed.

5. "CONFIGURATION": This button takes the operator to the Configuration screen.

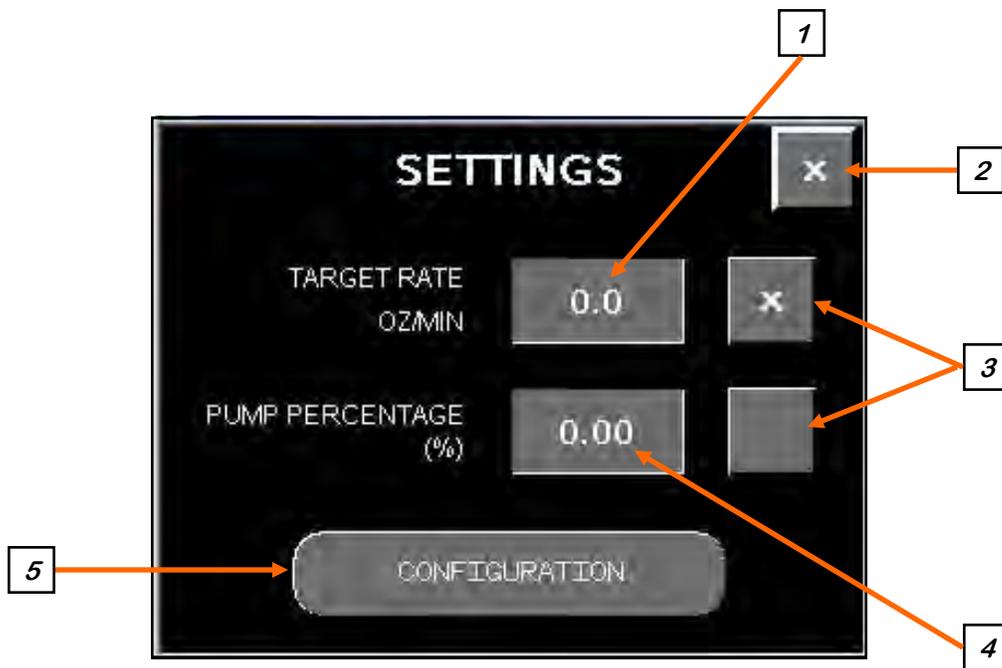


CONFIGURATION SCREEN

1. "FLOW METER TYPE": Pressing this button allows the operator to select the type of flow meter being used. Mass flow meter or Volumetric.

2. "# OF PUMP HEADS": Pressing this button allows the operator to select between a one, two or three head pump.


3. "UNIT OF MEASUREMENT": Allows the operator to switch between Standard or Metric units of measurement.

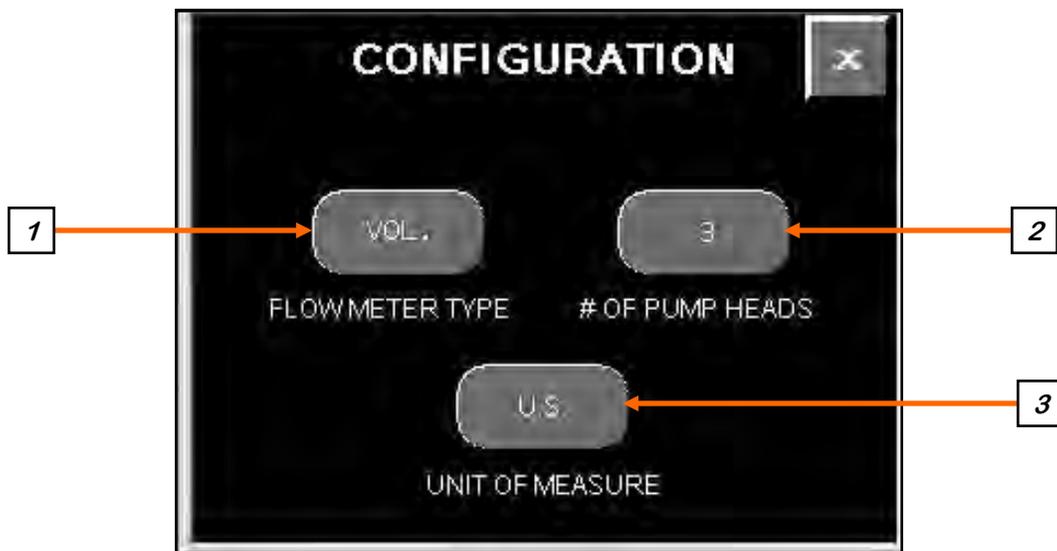

SEMI - AUTOMATED PUMP STAND


SELECT CHEMICAL SCREEN

1. **“SELECT CHEMICAL”**: Allows the operator to select which chemical to apply.
2. **“EDIT” Button**: This button takes the operator to the Edit Chemical screen.

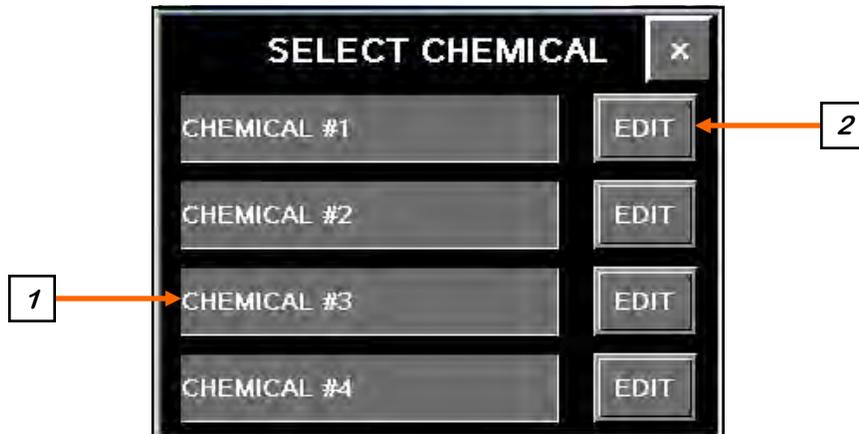

EDIT CHEMICAL SCREEN

1. **“CHEMICAL NAME”**: When this button is pushed a keypad appears (right) allowing the operator to enter or change a chemical name.
2. **“CALIBRATION FACTOR”**: When this button is pushed a numeric keypad appears allowing the operator to enter the (Multiplier) used for Flow Meter Calibration (see page 29).
3. **“CALCULATOR” Button**: This button takes the operator to the Multiplier Calculation screen. (see page 27)

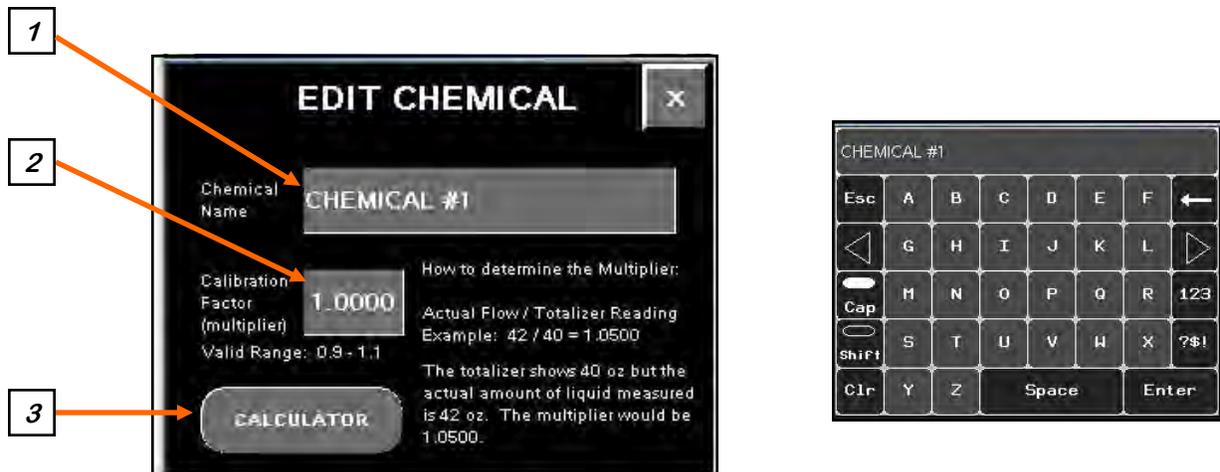

SEMI - AUTOMATED PUMP STAND



CALCULATOR SCREEN

1. "CALIBRATION TUBE": When this button is pushed a numeric keypad appears (below right) allowing the operator to enter the calibration tube reading while performing a flow meter calibration (see page 29).

2. "TOTALIZER": When this button is pushed a numeric keypad appears (below). Enter the amount that appears for the Totalizer (to the right) after calibration check enter number from the right.

3. "SAVE": Saves the information entered and calculates the multiplier and enters the data into the Calibration Factor Multiplier box (below left).

4. "CANCEL": Returns the operator to the Edit Chemical screen. Pressing the Cancel button before the Save button will not enter the Multiplier into the Factor Box.

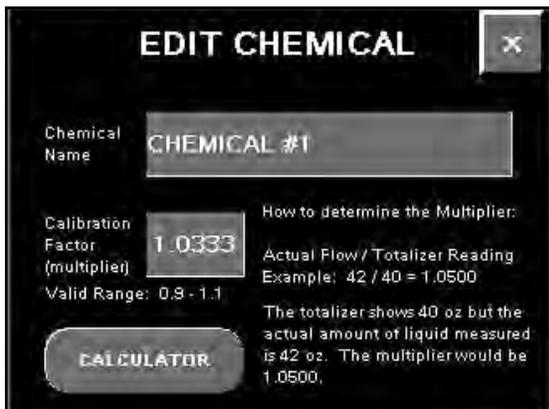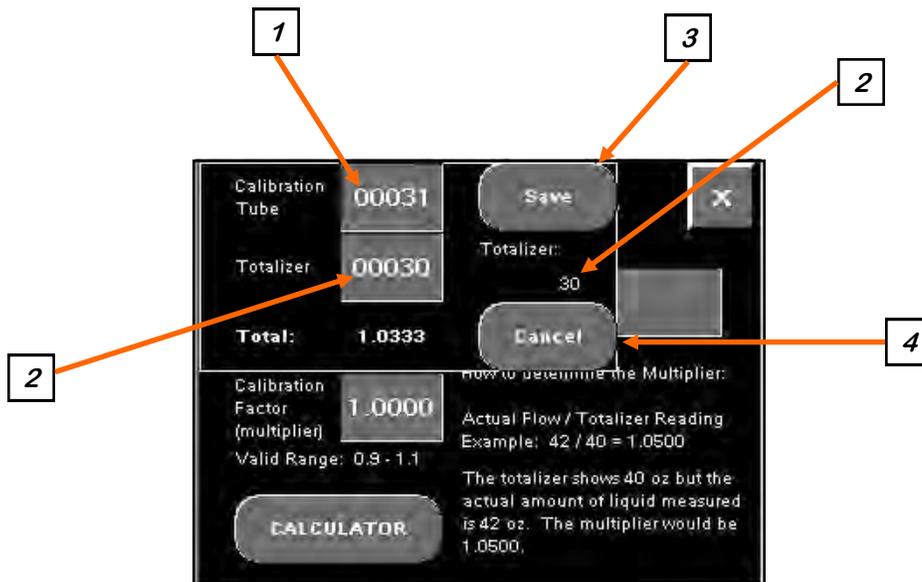


**SECTION
E**

CALIBRATION

PUMP CALIBRATION

1. Lock down the pump tubing in the pump head. (page 17)
2. Premix enough liquid for the amount of seed you are treating and pour into the chemical mix tank. It's always a good practice to mix up 20% extra slurry to help fill all the lines.
3. From the Main screen press the Chemical Status Box. From the Settings screen enter the number of ounces needed per minute per hundred pounds of seed as the Target Rate. Then, press the "EDIT" button and verify that the Calibration Factor is set to one. Return to the Main screen and select the Select Chemical button. From the Select Chemical screen choose the type of chemical.
4. Set the return valves to Mix Tank for recirculation. Turn the ON/OFF switch for the mix tank motor to the "ON" position. Run it for 15 minutes to ensure that the chemical mixture within the mix tank is blended completely and any air is removed from the system.

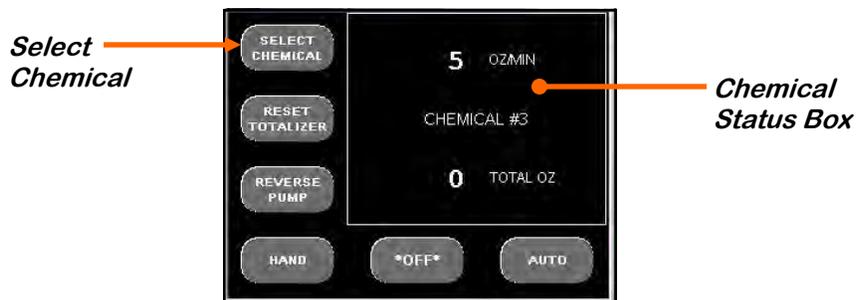

*Enter in
Ounces per
cwt. here*


*Choose
chemical
name here*



FLOW METER CALIBRATION

Due to the composition of some types of chemicals, additional flow meter calibration may be required. It is recommended that, like other calibration devices, the flow meter(s) are checked regularly and calibrated when needed. When calibrating the flow meter(s), each chemical slurry must be checked and adjusted for.

1. To begin the calibration process, fill the appropriate mix tank with the slurry that is going to be used for this calibration.
2. Turn the ON/OFF switch for the mix tank motor to the "ON" position. From the Main screen select the Chemical Status Box. Enter a value for the Pump Percentage speed (Example 20) and check the box to the right. Return to the Main screen, press the "HAND" button and ensure that the valves are set to Mix Tank for recirculation. Let the system run in recirculation mode for 15 minutes. This will remove any air from the system.
3. Ensure that the correct chemical has been chosen.
4. Place the bottom return valve to "MIX TANK/CALIBRATION TUBE". The valve is located on top of the pump stand (right). Place the top valve to the "CALIBRATION TUBE" position. Once the liquid in the Calibration Tube reaches zero press "HAND" or "OFF" to stop the pump. Press the "TOTALIZER" button to zero out the Totalizer. Press the "HAND" button and start the stopwatch simultaneously. Stop the pump when the stopwatch reaches one minute. Note the total ounces of chemical that is in the calibration tube.
5. Push the Calculator button. It is located in the bottom left corner of the Edit Chemical screen. Enter the number of the ounces in the calibration tube box. Between the Save and Cancel button is the number of ounces read by the flow meter. Enter that amount in the Totalizer box and press SAVE. The system automatically calculates and places the amount in the Calibration Factor (Multiplier) box.
6. Repeat the process as necessary and for each different chemical slurry used.

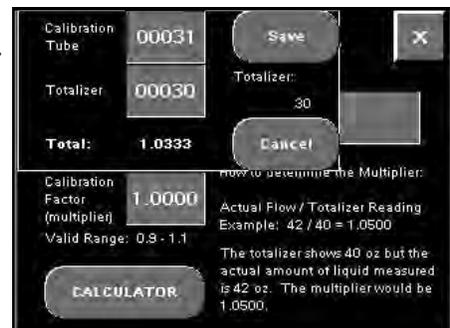

SECTION
F**TROUBLESHOOTING****TROUBLESHOOTING**

Below is a table describing the most frequent problems and solutions with the USC Semi - Automated Pump Stand. For further assistance, contact your local USC dealer.

Problem	Possible Cause	Solution
Pump is fluctuating.	<ol style="list-style-type: none"> 1. Restriction in tubing 2. Filter is plugged or missing gasket. 3. Hoses are worn out. 	<ol style="list-style-type: none"> 1. Flush tubing and check filter for any restrictions. 2. Clean filter and check for gasket. 3. Replace hoses.
Pump will not turn off in "AUTO" when seed runs out.	<ol style="list-style-type: none"> 1. Proximity switch is dirty. 2. Proximity switch is set too sensitive. 	<ol style="list-style-type: none"> 1. Clean proximity switch. 2. Adjust the pump proximity switch sensitivity by turning adjustment screw counter-clockwise.
Pump will not turn on in "AUTO".	<ol style="list-style-type: none"> 1. Proximity switch is not staying covered. 2. Proximity switch is not sensitive enough. 3. HMI screen not set to "AUTO". 4. Auxiliary cable not hooked up. 	<ol style="list-style-type: none"> 1. Make sure proximity switch is staying covered with seed. 2. Adjust pump proximity switch sensitivity by turning the adjustment screw clockwise. 3. Set HMI screen to "AUTO". 4. Attach Auxiliary cable from control box to treater control box.
Mix Motor will not start	<ol style="list-style-type: none"> 1. Power cord not plugged in. 	<ol style="list-style-type: none"> 1. Plug in power cord.

MAINTENANCE

SECTION G

Proper maintenance of the Semi - Automated Pump Stand is critical for peak performance, reliability and accuracy of this system. The following is a guideline for the type of maintenance and servicing that should be performed on this unit. Your environment and uses may require additional maintenance and service beyond this list to assure a reliable and safe unit. The operator of this unit has ultimate responsibility to identify areas of concern and rectify them before they become a hazard or safety issue. There is no substitute for a trained, alert operator.



Do not put this unit into operation with any questionably maintained parts. Poor performance or a hazard may occur.

PUMPS AND PLUMBING

- Check pump in forward and reverse.
- Make sure pump heads open and close smoothly.
- Inspect tubing and for uneven wear. Replace pump tubing often to ensure high flow rates can be met.
- Tighten hose clamps and check filter. Clean filter frequently to avoid blockages
- Flush flow meter with clean water frequently to avoid chemical buildup.

MIX TANK

- Check motor.
- Check for any play in the mix tank shaft.
- Check valves, fittings, and plug on bottom of tank for leaks.
- Check chemical line tubing for abnormal wear.

ELECTRICAL PANEL

- Check quick connects on end of Auxiliary cord.
- Check and tighten wire connections.
- Check relay and fuse holder.
- Check power cords for cuts or frays and ensure ground is present.

**SECTION
H****STORAGE**


When storing the Semi - Automated Pump Stand for long periods of time, the following procedure must be followed to reduce the chance of rust, corrosion and fatigue of the pump stand. You can also use these steps when storing the machine for the winter.



A dust mask and protective rubber gloves shall be used when cleaning the machine.

LIQUID SYSTEM

1. Make certain the inside of the tank is completely drained of chemical residue and thoroughly flush the inside of the tank with clean water.
2. Remove and clean the filter.
3. Pump clean water through all areas of the plumbing including the mix tank, flow meter, and valves.
4. Open all drain points, valves, and filter to let as much of the liquid drain as possible.
5. If the pump stand will be exposed to possible freezing temperatures, the final flush of the system should be made with a non freezable liquid. Or use compressed air to blow the lines out from any moisture.
6. Release pump heads (right) and remove tubing to prevent any unnecessary wear.

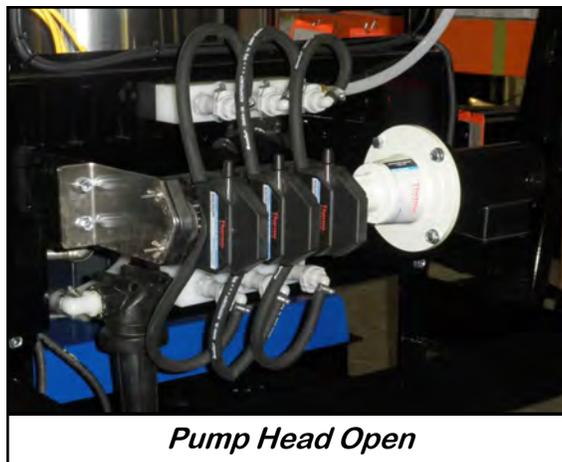

Pump Head Open


NOTES

[Empty rectangular box for notes]

SECTION
I

MECHANICAL DRAWINGS

Semi - Automated Pump Stand - Base Frame (05-03-1066)

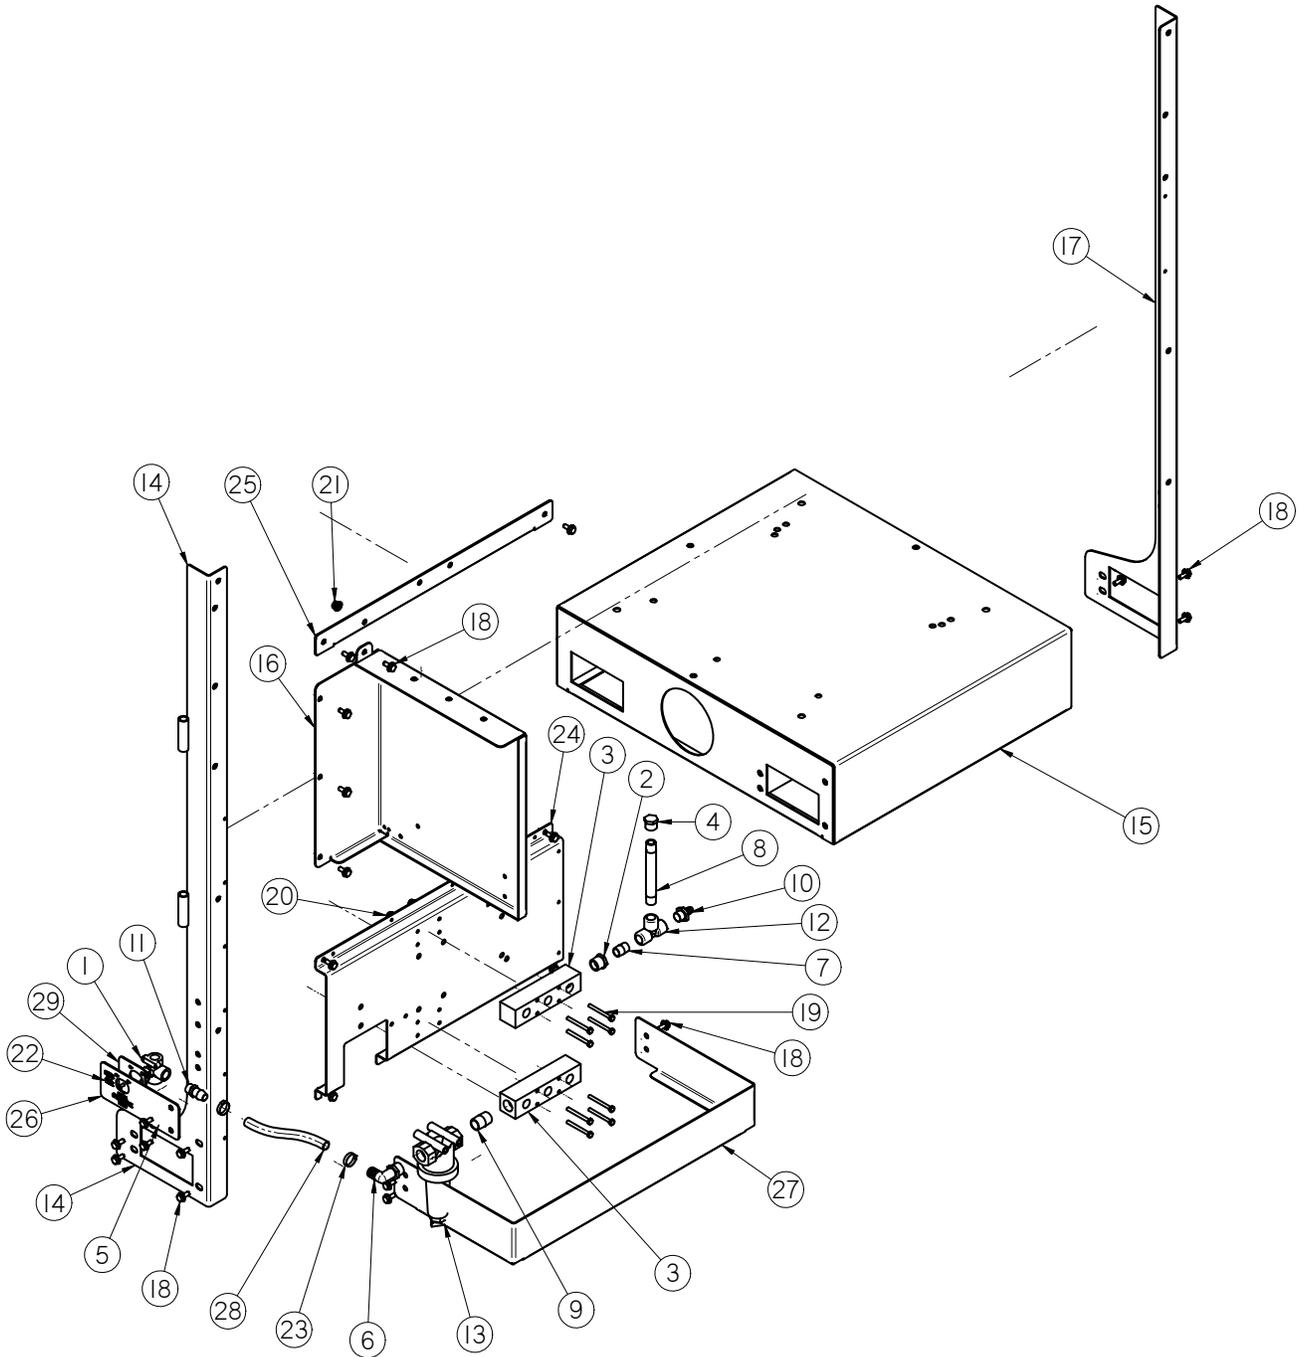


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - Base Frame (05-03-1066)

Item #	Part #	Description	Qty
1	02-02-0007	VLV BALL .500 NPT 3WAY BRSS	1
2	02-04-0008	BUSHING .750-14 NPT, REDUCER .500-14 NPT	1
3	02-05-0043	FTTG MANIFOLD UHMW 1 IN 3 OUT	2
4	02-05-0086	FTTG END CAP .500 NPT BP	1
5	02-06-0014	1/2-14 NPT, 3/4 BARB, 90 DEG. WP	1
6	02-06-0015	BARB, .750-14 NPT X .750 90DEG WP	1
7	02-07-0008	FTTG NIP .500 NPT X 1.125 TBE BLK	1
8	02-07-0060	FTTG NIP .500 NPT X 6.00 TBE PVC	1
9	02-07-0070	FTTG NIP .750 NPT X 1.50 TBE SS	1
10	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	1
11	02-08-0011	1/2-14 NPT, 3/4 BARB, STRAIGHT BP	1
12	02-09-0005	FTTG TEE .500 NPT PPE	1
13	02-12-0011	FLTR TEE PPE .750 NPT 16 MESH BANJO	1
14	05-03-1052	WDMT SMALL PUMPSTAND LH UPRIGHT	1
15	05-03-1053	WDMT SMALL PUMPSTAND BASE BOX	1
16	05-03-1064	WDMT PANEL MNT PUMPSTD	1
17	05-03-1074	WDMT SMALL PUMPSTAND RH UPRIGHT	1
18	06-01-0124	BOLT, FLG .375-16 UNC ZP GRADE 5; 3/4" LG	24
19	06-01-0192	BOLT .250-20 X 2.50 ZP GR5	8
20	06-03-0013	NUT,LOCK, FLG .250-20 ZP SERRATED	8
21	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	1
22	06-06-0020	SRCW, PAN HD, 10-24 X .500 ZP	2
23	06-07-0030	HOSE CLAMP ONE EAR 1.004-1.126	2
24	102200	BRKT PUMP ALL HEADS PUMPSTD	1
25	10220E	PLT XBEAM SUPP VLV PUMPSTD	1
26	102290	PLT LABEL SOURCE PUMPSTD	1
27	1022AA	BRKT FORKLIFT GUARD PUMPSTD	1
28	1022AB	1022AB 02-03-0006 8.25IN LONG	1
29	1022AC	PLT SPACER VLV SOURCE MOUNT	1

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - Single Peristaltic Pump Head (13-04-0105)

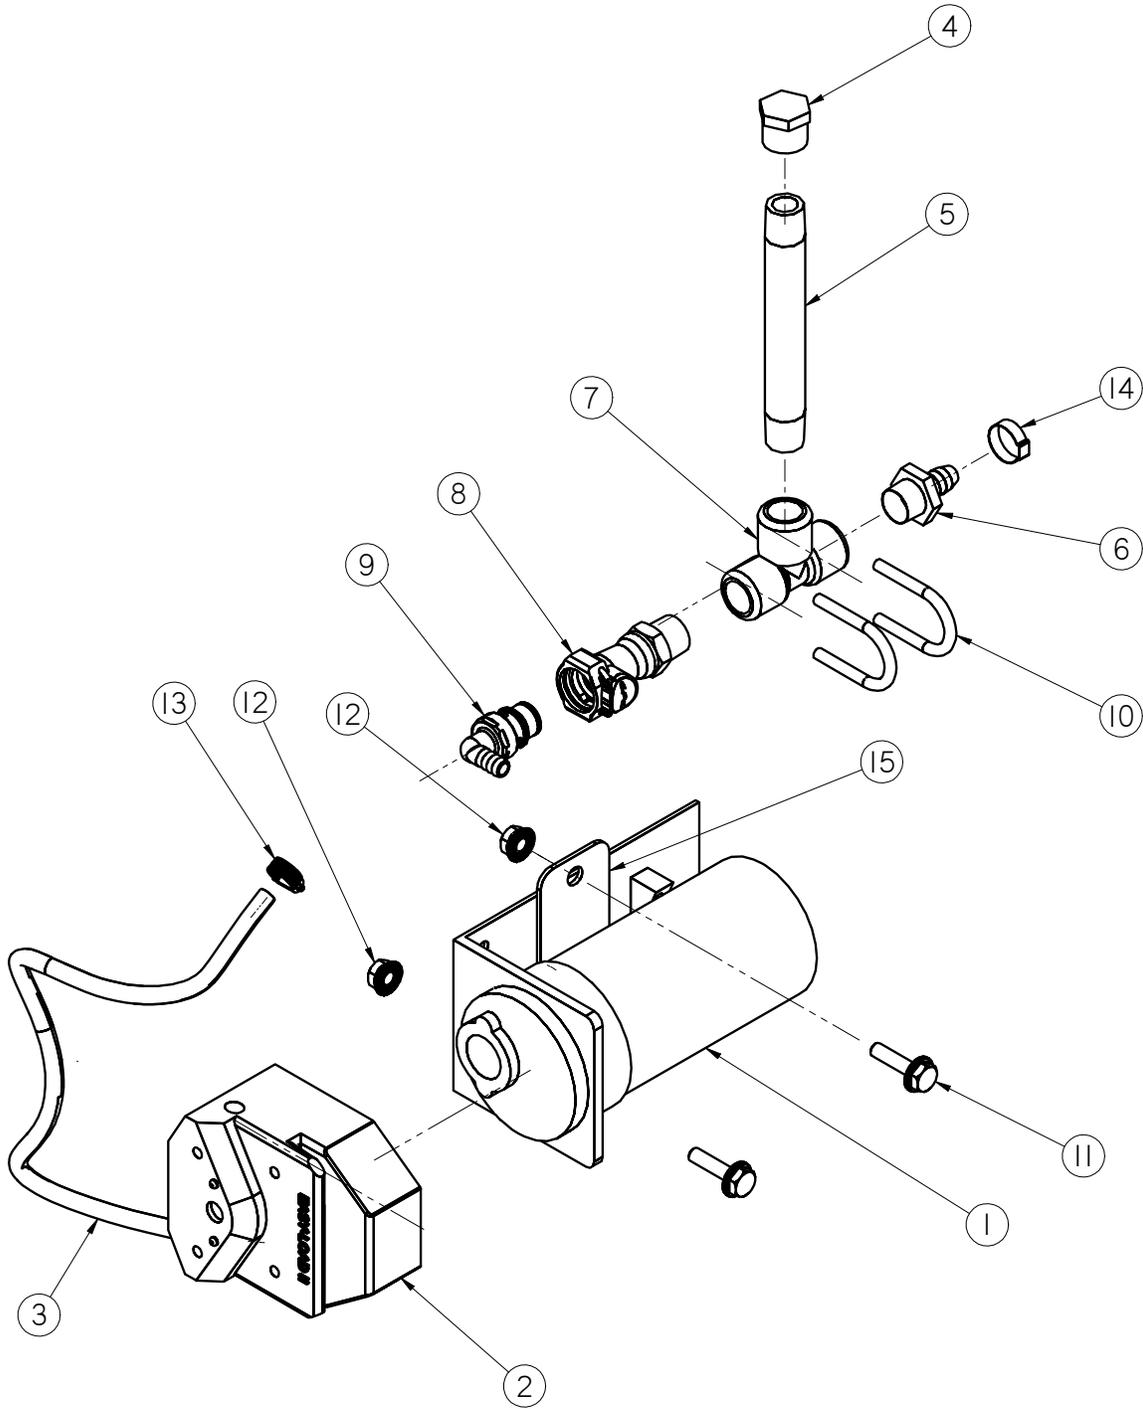


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - Single Peristaltic Pump Head (13-04-0105)

Item #	Part #	Description	Qty
1	01-01-0010	MTR .1HP 6-600RPM 90VDC	1
2	02-01-0005	PUMP HEAD PRST MF LS 115V 600RPM	1
3	02-03-0001	TUBE MASTERFLEX PUMPHEAD	4
4	02-05-0086	FTTG END CAP .500 NPT BP	1
5	02-07-0060	FTTG NIP .500 NPT X 6.00 TBE PVC	1
6	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	1
7	02-09-0005	FTTG TEE .500 NPT PPE	1
8	02-15-0016	FTTG CPLG .500 NPT QCK DISC BODY	1
9	02-15-0022	FTTG CPLG .375 BARB QCK DISC INSERT	1
10	06-01-0120	U BOLT 1/4-20 1-1/8 INSIDE 2" LG	2
11	06-01-0189	BOLT, FLG .375-16 UNC ZP GRADE 5; 1-1/4" LG	2
12	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	2
13	06-07-0005	CLMP HOSE .219 TO .625 X .313W ZP	2
14	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	1
15	102276	BRKT PUMP MOUNT PUMPSTD	1

SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - Dual Peristaltic Pump Head (13-04-0104)

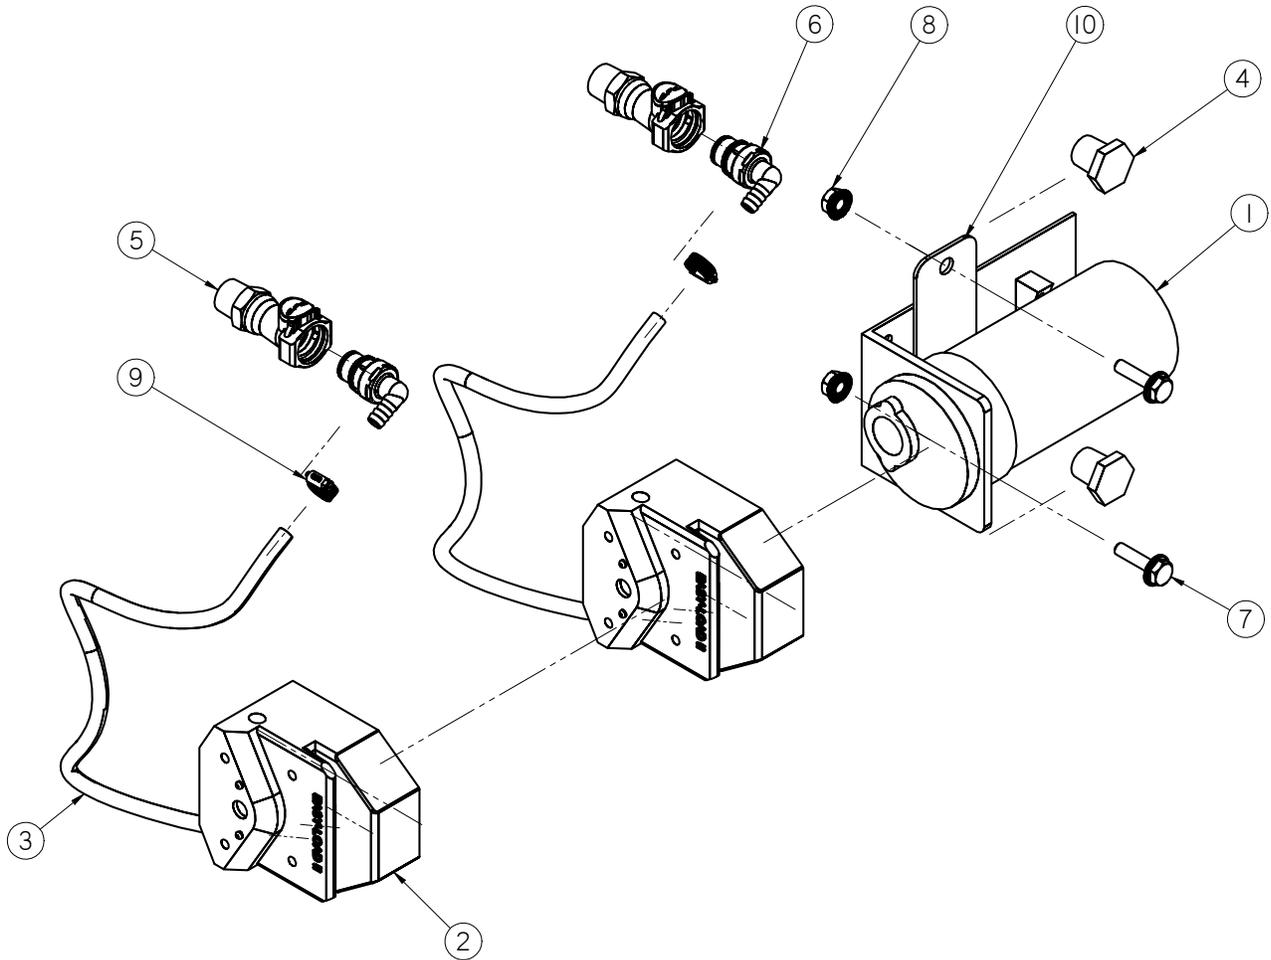

Item #	Part #	Description	Qty
1	01-01-0010	MTR .1HP 6-600RPM 90VDC	1
2	02-01-0005	PUMP HEAD PRST MF LS 115V 600RPM	2
3	02-03-0001	TUBE MASTERFLEX PUMPHEAD	5
4	02-14-0002	1/2-14 NPT,PLUG BP	2
5	02-15-0016	FTTG CPLG .500 NPT QCK DISC BODY	4
6	02-15-0022	FTTG CPLG .375 HB X 90 QCK DISC INSERT	4
7	06-01-0189	BOLT, FLG .375-16 UNC ZP GRADE 5; 1-1/4" LG	2
8	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	2
9	06-07-0005	CLMP HOSE .219 TO .625 X .313W ZP	4
10	102276	BRKT PUMP MOUNT PUMPSTD	1

SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - Triple Peristaltic Pump Head (13-04-0103)

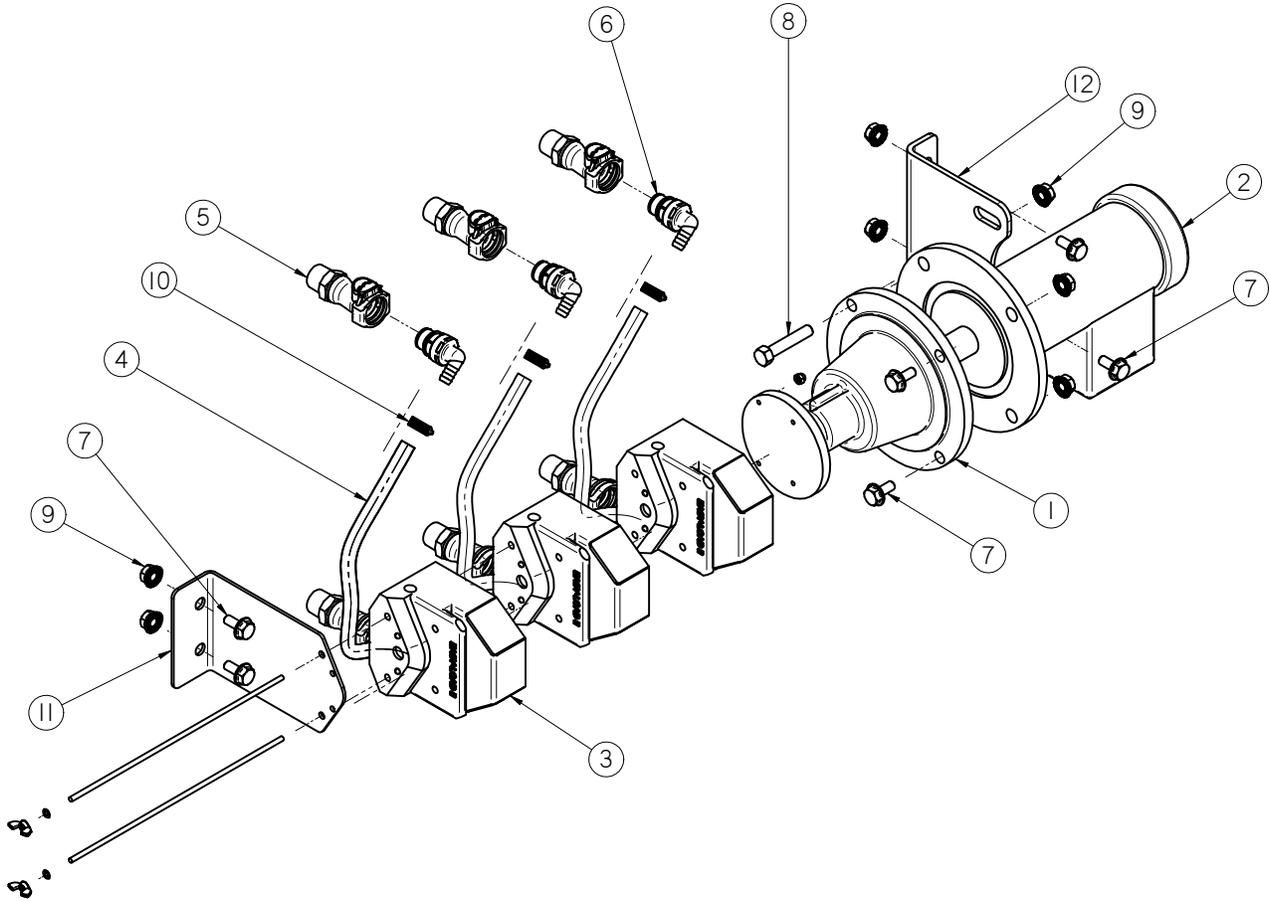

Item #	Part #	Description	Qty
1	01-01-0066	SPEED REDUCER, 3.7 TO 1	1
2	01-01-0160	MTR .25HP 2500 RPM 34 90VDC	1
3	02-01-0005	PUMP HEAD PRST MF LS 115V 600RPM	3
4	02-03-0001	HOSE MF .375 NPRN BLK - LS35 .31 ID	6
5	02-15-0016	FTTG CPLG .500 NPT QCK DISC BODY	6
6	02-15-0022	FTTG CPLG .375 HB X 90 QCK DISC INSERT	6
7	06-01-0124	BOLT, FLG .375-16 UNC ZP GRADE 5; 3/4" LG	6
8	06-01-0137	BOLT .375-16 X 2.00 ZP GR5 FULL THRD	2
9	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	8
10	06-07-0005	CLMP HOSE .219 TO .625 X .313W ZP	6
11	102213	BRKT 3PUMPHEAD MNT PUMPSTD	1
12	102214	BRKT 3HEAD MOTOR MNT PUMPSTD	1

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - Calibration Tube (13-04-0106)

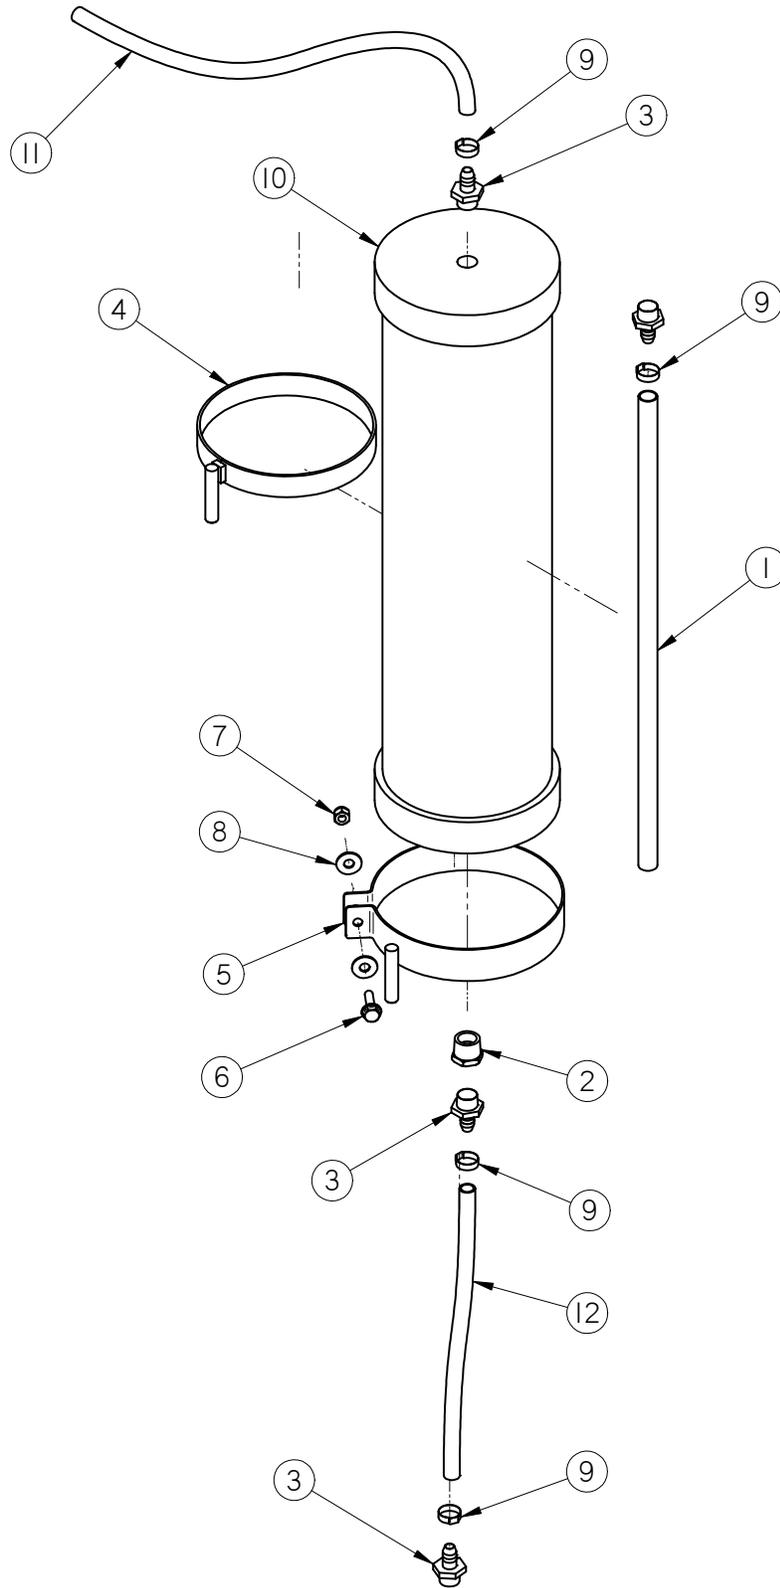


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - Calibration Tube (13-04-0106)

Item #	Part #	Description	Qty
1	02-03-0005	TUBE,CALIBRATION TUBE INSIDE	1
2	02-04-0008	BUSHING .750-14 NPT, REDUCER .500-14 NPT	1
3	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	4
4	05-08-0006	WDMT,INOC.BRK,SM	1
5	05-08-0007	WDMT,BRK,INOC LG	1
6	06-01-0189	BOLT, FLG .375-16 UNC ZP GRADE 5; 1-1/4" LG	1
7	06-03-0003	NUT NYL LOCK .375-16 ZP GR5	1
8	06-05-0004	WSHR FLAT .375 ZP	2
9	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	4
10	07-02-0006	CALIBRATION TUBE,10K ML - 2005	1
11	102A39	TUBE SOL VLV TO CAL TUBE PUMPSTD	1
12	102A3A	TUBE CAL TUBE TO VLV PUMPSTD	1

SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - Dry Lock Fittings (13-10-0017)

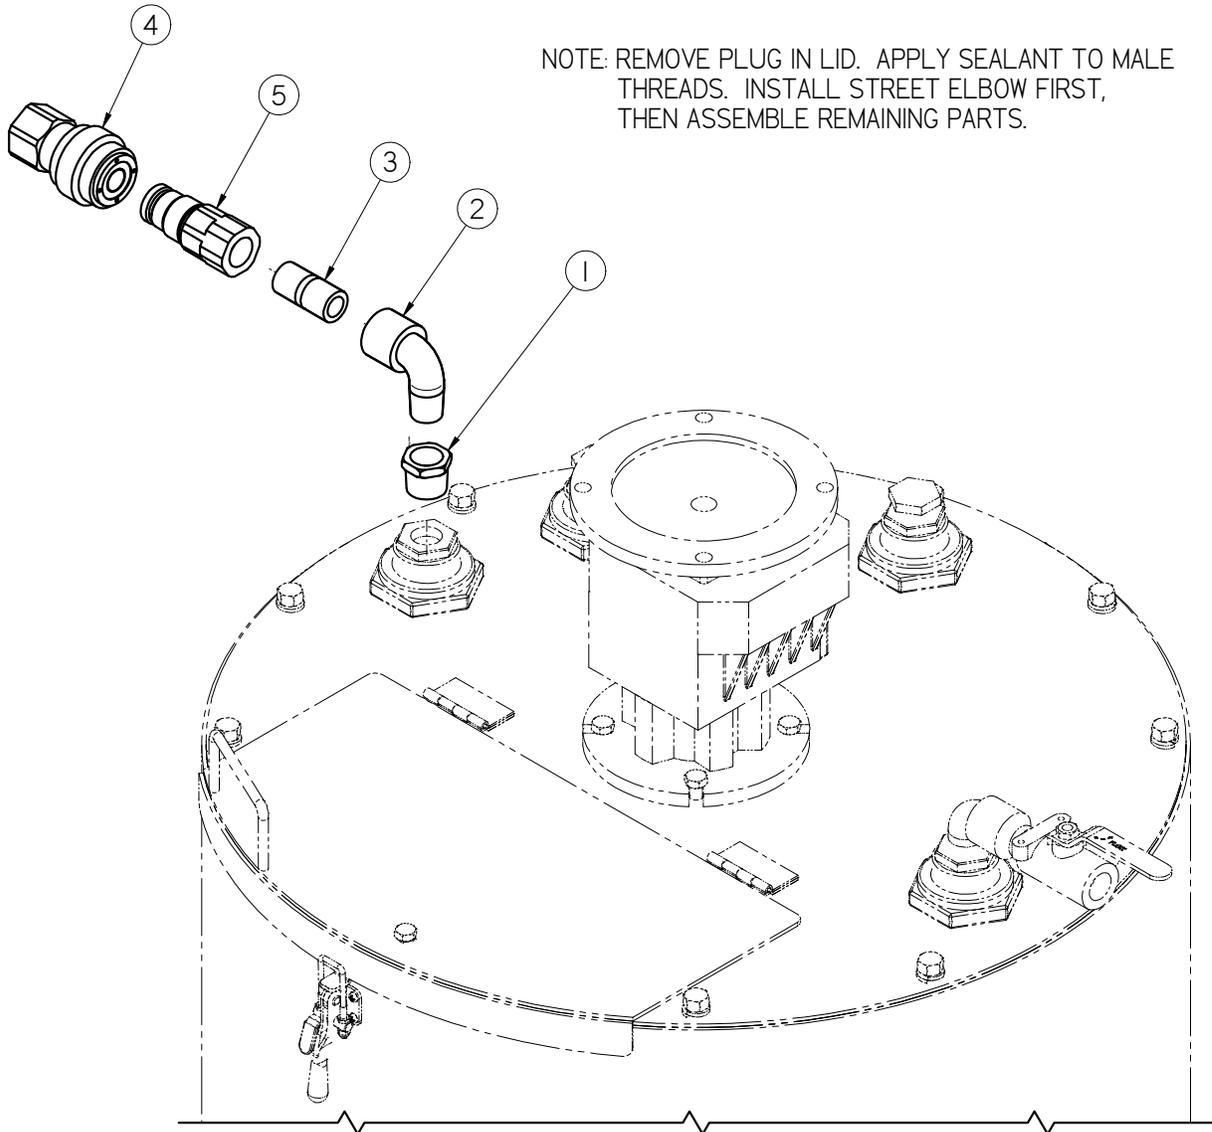

Item #	Part #	Description	Qty
1	02-04-0024	BUSH .750-14 NPT .500-14 NPT BP	1
2	02-06-0017	1/2-14 NPT,SL 90 DEG. BP	1
3	02-07-0009	FTTG NIP .500 NPT X 1.75 TBE BLK	1
4	02-15-0035	FTTG CPLG 0.50 NPT FM PARKER POLY	1
5	02-15-0036	FTTG CPLG 0.50 NPT ML PARKER POLY	1

SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - Scale Assembly (05-03-1069)

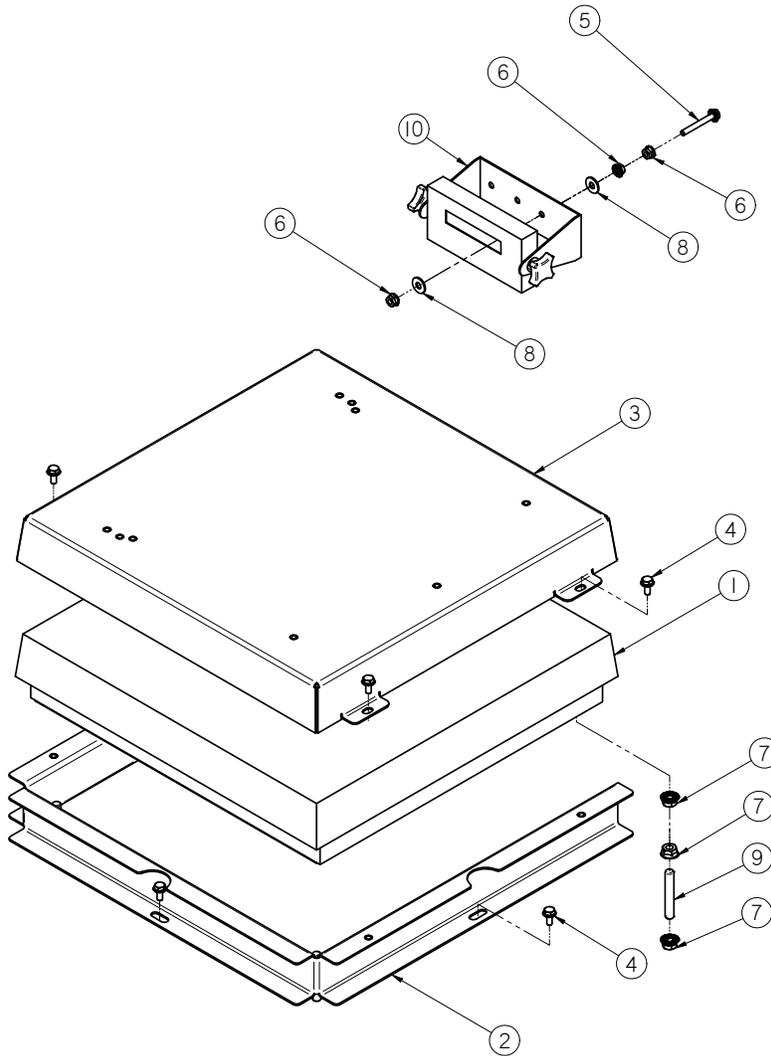

Item #	Part #	Description	Qty
1	03-19-0055	SCL CARDINAL EB-1024 24 X 24 X 1000	1
2	05-03-1072	WDMT SPACER PUMPSTD	1
3	05-03-1073	WDMT SCALE LID PUMPSTD	1
4	06-01-0124	BOLT, FLG .375-16 UNC ZP GRADE 5; 3/4" LG	7
5	06-01-0204	BOLT FLG .375-16 X 2.50 ZP GR5 FTH	1
6	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	3
7	06-03-0015	NUT LOCK FLG .500-13 ZP GR5	12
8	06-05-0004	WSHR FLAT .375 ZP	2
9	06-14-0018	.500-13 THD RD CS 3IN LONG	4
10	PART OF 03-19-0055	SCALE DISPLAY	1

SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - Mass Flow Meter (05-03-1067)

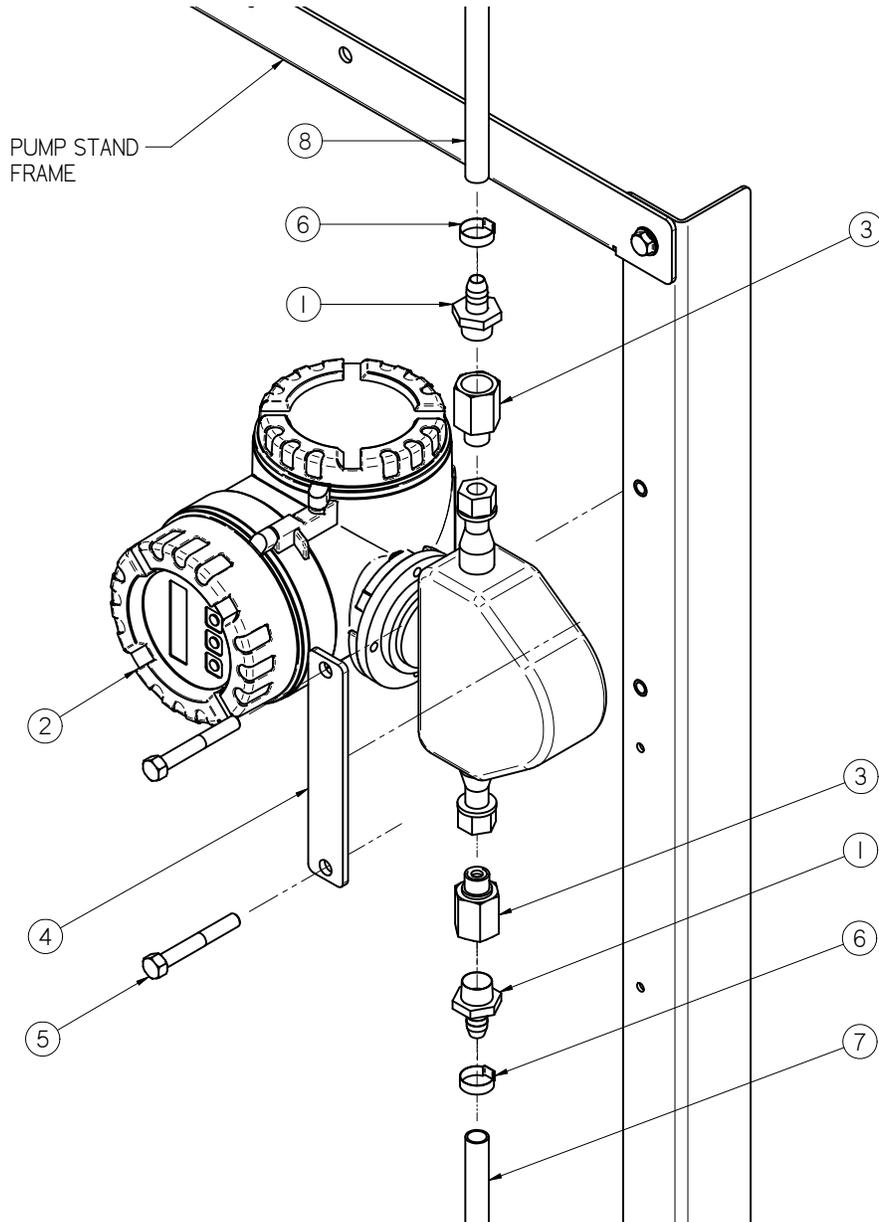

Item #	Part #	Description	Qty
1	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	2
2	03-18-0012	E+H 83S FLOW METER	1
3	03-18-0021	FTTG ADPTR 1/2" VCO X 1/2" FPT E+H	2
4	05-10-3413	BRACKET FLMT CLAMP E&H 83E	1
5	06-01-0116	BOLT .375-16 X 2.75 ZP GR5	2
6	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	2
7	1022AE	MASS FLMT TO PUMPS	1
8	102342	MASS FLMT TO CNTLS	1

SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - Volumetric Flow Meter (05-03-1068)

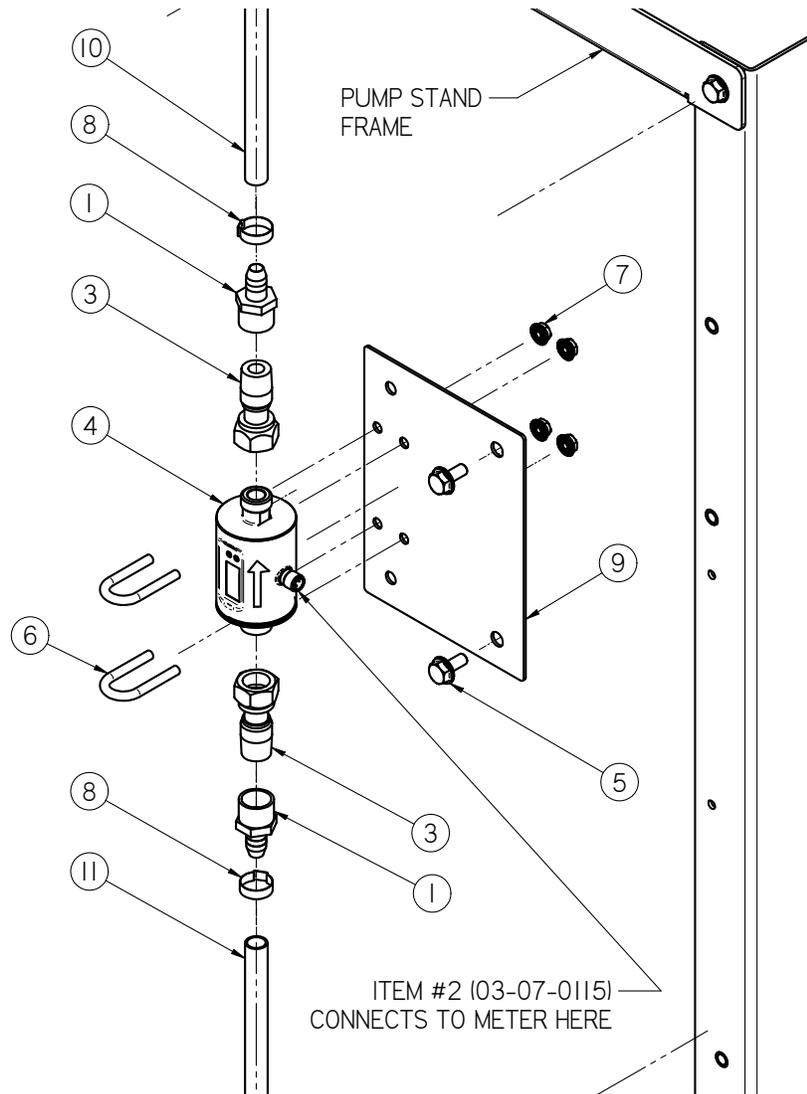

Item #	Part #	Description	Qty
1	02-08-0026	FTTG STGHT .500HB X .500NPT FM NYL	2
2	03-07-0115	CORD MOLDED M12 IFM EVC001	1
3	03-18-0020	FTTG ADPTR G1/2 TO 1/2NPT ML IFM	2
4	03-18-0025	FLMT IFM EFECTOR SM6000 AE 1/2 IN	1
5	06-01-0124	BOLT, FLG .375-16 UNC ZP GRADE 5; 3/4" LG	2
6	06-01-0199	BOLT U .313-18 X 1.00 X .375 ZP GR5	2
7	06-03-0013	NUT, LOCK, FLG .250-20 ZP SERRATTED	4
8	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	2
9	1029CF	BRKT MNT	1
10	102A3B	VOL FLMT TO CNTLS	1
11	102A3C	VOL FLMT TO PUMPS	1

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 30 Gallon Stainless Steel Tank (04-03-0172)

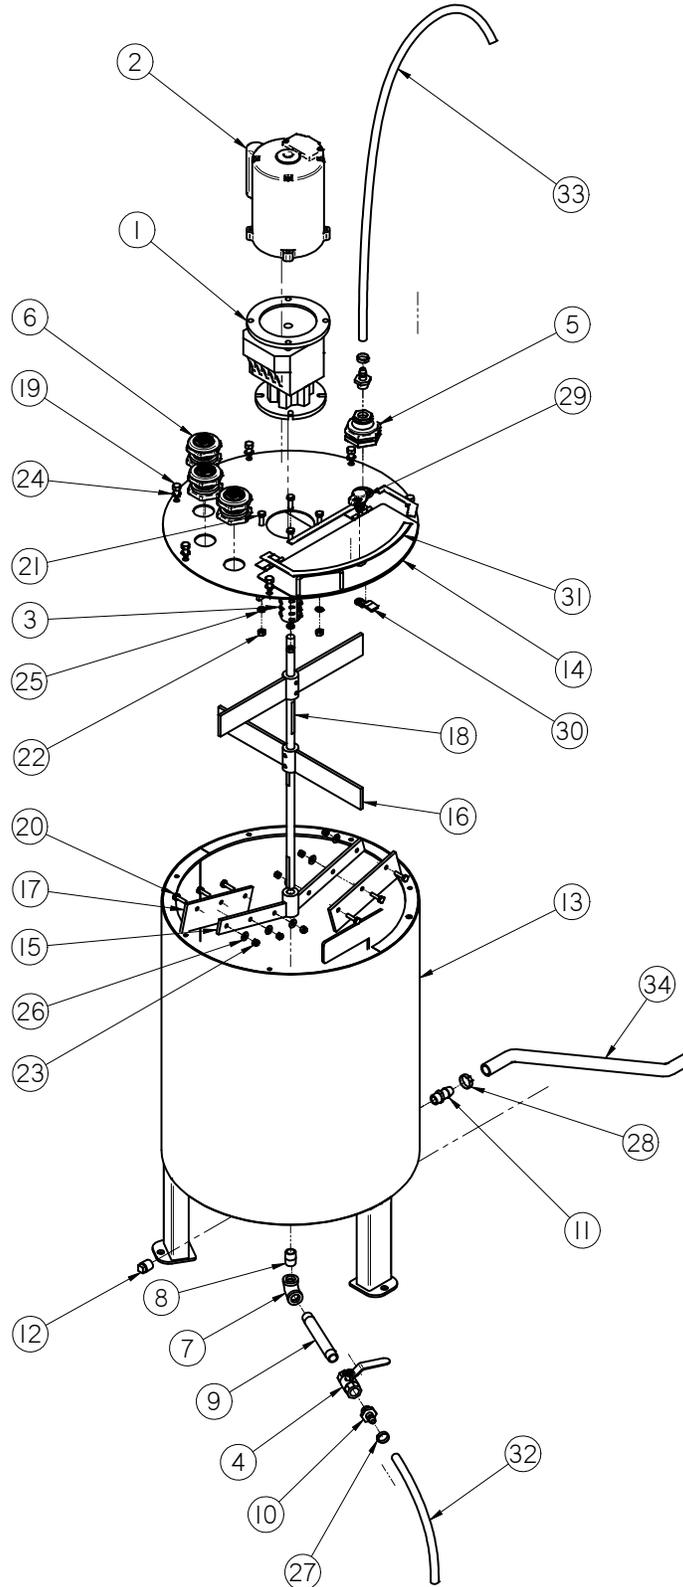


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 30 Gallon Stainless Steel Tank (04-03-0172)

Item #	Part #	Description	Qty
1	01-01-0039	GBOX IL 61.8:1 56C OTP 56C INP	1
2	01-01-0080	MTR .33HP 1725RPM 56C 1PH TEFC	1
3	01-07-0015	CPLG CLPN .625 X .750 X 1.50OD SS	1
4	02-02-0006	.500-14 NPT X 2-WAY VALVE	1
5	02-05-0028	FTTG .500 NPT DBL THD PPE BULKHEAD	1
6	02-05-0045	FTTG .750 NPT DBL THD PPE BULKHEAD	3
7	02-06-0012	ELBOW, .500-14 NPT, 90 DEG. SS	1
8	02-07-0007	FTTG NIP .500 NPT X 1.125 TBE SS	1
9	02-07-0015	FTTG NIP .500 NPT X 6.00 TBE SS	1
10	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	2
11	02-08-0011	1/2-14 NPT, 3/4 BARB, STRAIGHT BP	1
12	02-14-0001	FTTG PLUG SQHD .500 NPT SS	1
13	05-03-1088	WDMT 30GAL CHEM TNK LOCK LID	1
14	05-03-1089	WDMT 30GAL REMV TOP LOCK LID	1
15	05-04-0005	WDMT 27GAL STIR ARM LOWER	1
16	05-04-0011	WDMT 27GAL STIR ARM MIDDLE	2
17	05-10-0799	PDL 27GAL WIPER	2
18	05-11-0349	30-GAL TANK STIR ROD	1
19	06-01-0042	BOLT, .375-16 X .750 18-8 SS	6
20	06-01-0051	BOLT .250-20 X 1.00 SS 316	6
21	06-01-0060	BOLT, .312-18 UNC 316 SS; 1.00" LG	4
22	06-02-0017	NUT FULL .313-18 SS 18-8	4
23	06-03-0007	NUT NYL LOCK .250-20 SS 18-8	6
24	06-04-0008	WASHER, .375 LOCK 316 SS	6
25	06-04-0010	WASHER, .3125 LOCK 18-8 SS	4
26	06-05-0002	WASHER, .250 FLAT 316 SS	6
27	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	2
28	06-07-0030	HOSE CLAMP ONE EAR 1.004-1.126	1
29	06-09-0075	KNOB WING LATCH	1
30	06-09-0076	KNOB WING CAM	1
31	06-10-0001	SEAL,CHARCAOL TANK	1
32	1022B2	DRAIN HOSE PUMP STAND	1
33	102346	HOSE SOL VLV TO TANK	1
34	102C1B	HOSE TANK TO VLV	1

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 60 Gallon Stainless Steel Tank (04-03-0173)

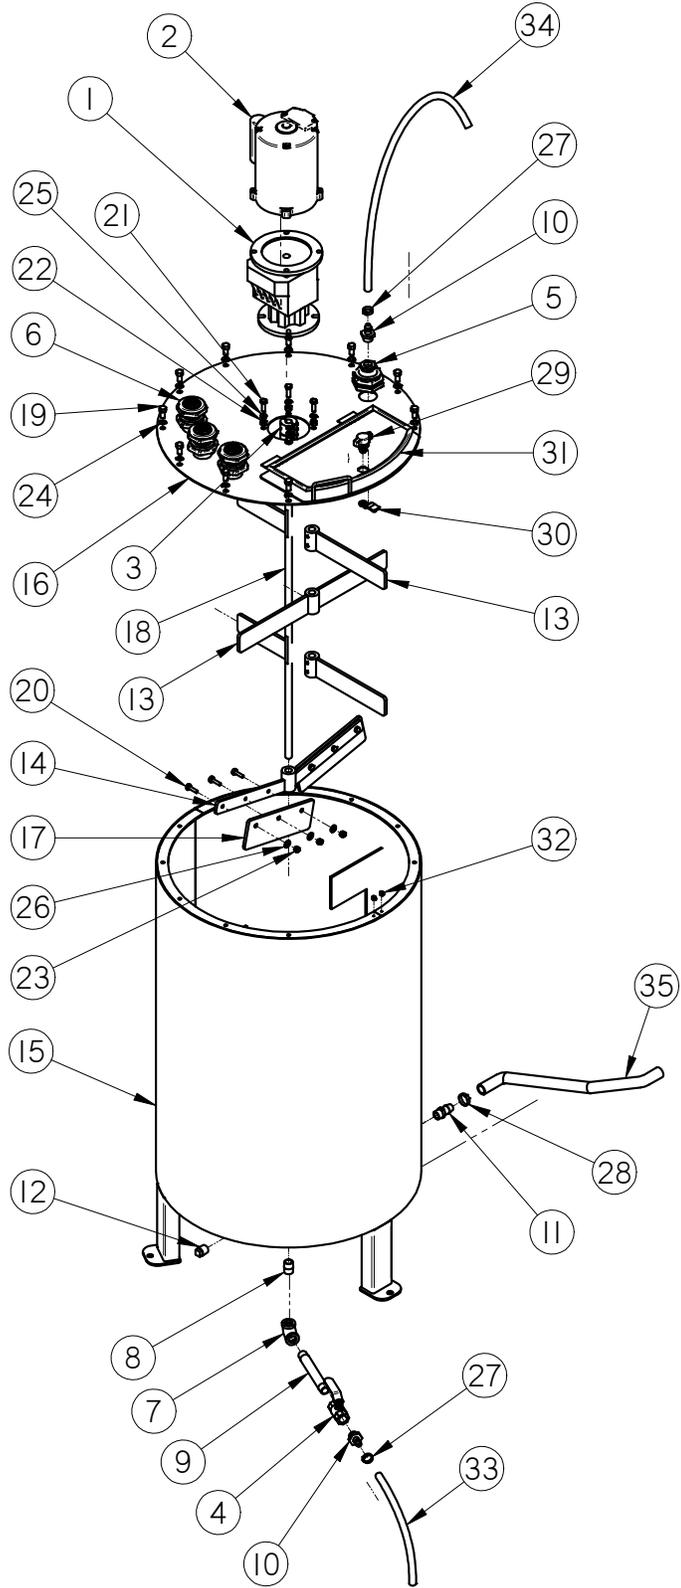


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 60 Stainless Steel Tank (04-03-01)


Item #	Part #	Description	Qty
1	01-01-0039	GBOX IL 61.8:1 56C OTP 56C INP	1
2	01-01-0080	MTR .33HP 1725RPM 56C 1PH TEFC	1
3	01-07-0015	CPLG CLPN .625 X .750 X 1.50OD SS	1
4	02-02-0006	VLV BALL .500 NPT 2WAY BRSS	1
5	02-05-0028	FTTG .500 NPT DBL THD PPE BULKHEAD	1
6	02-05-0045	FTTG .750 NPT DBL THD PPE BULKHEAD	3
7	02-06-0012	ELBOW, .500-14 NPT, 90 DEG. SS	1
8	02-07-0007	FTTG NIP .500 NPT X 1.125 TBE SS	1
9	02-07-0015	FTTG NIP .500 NPT X 6.00 TBE SS	1
10	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	2
11	02-08-0011	1/2-14 NPT, 3/4 BARB, STRAIGHT BP	1
12	02-14-0001	FTTG PLUG SQHD .500 NPT SS	1
13	05-03-0069	WDMT 50GAL MIDDLE STIR ARM	3
14	05-03-0070	WDMT 50GAL LOWER STIR ARM	1
15	05-03-1078	WDMT BASE 60GAL TANK	1
16	05-03-1079	WDMT 60GAL REMOVABLE TOP 2 HOLE	1
17	05-10-0878	PDL 50GAL WIPER	2
18	05-11-0341	ROD 60GAL DRV	1
19	06-01-0042	BOLT, .375-16 X .750 18-8 SS	10
20	06-01-0051	BOLT .250-20 X 1.00 SS 316	6
21	06-01-0060	BOLT, .312-18 UNC 316 SS; 1.00" LG	4
22	06-02-0017	NUT FULL .313-18 SS 18-8	4
23	06-03-0007	NUT NYL LOCK .250-20 SS 18-8	6
24	06-04-0008	WSHR LOCK SPLT .375 SS 18-8	10
25	06-04-0010	WSHR LOCK SPLT .313 SS 18-8	4
26	06-05-0002	WSHR FLAT .250 X .625OD SS 18-8	6
27	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	2
28	06-07-0030	HOSE CLAMP ONE EAR 1.004-1.126	1
29	06-09-0075	KNOB WING LATCH	1
30	06-09-0076	KNOB WING CAM	1
31	06-10-0001	SEAL RBBR BULBS CHAR .500 X .250	1
32	06-12-0011	3/16 X .450" LONG POP RIVET	2
33	1022B2	DRAIN HOSE PUMP STAND	1
34	1022C0	HOSE SOL VLV TO TANK	1
35	102C1C	HOSE TANK TO VLV	1

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 30 Gallon Poly Tank (04-03-0161)

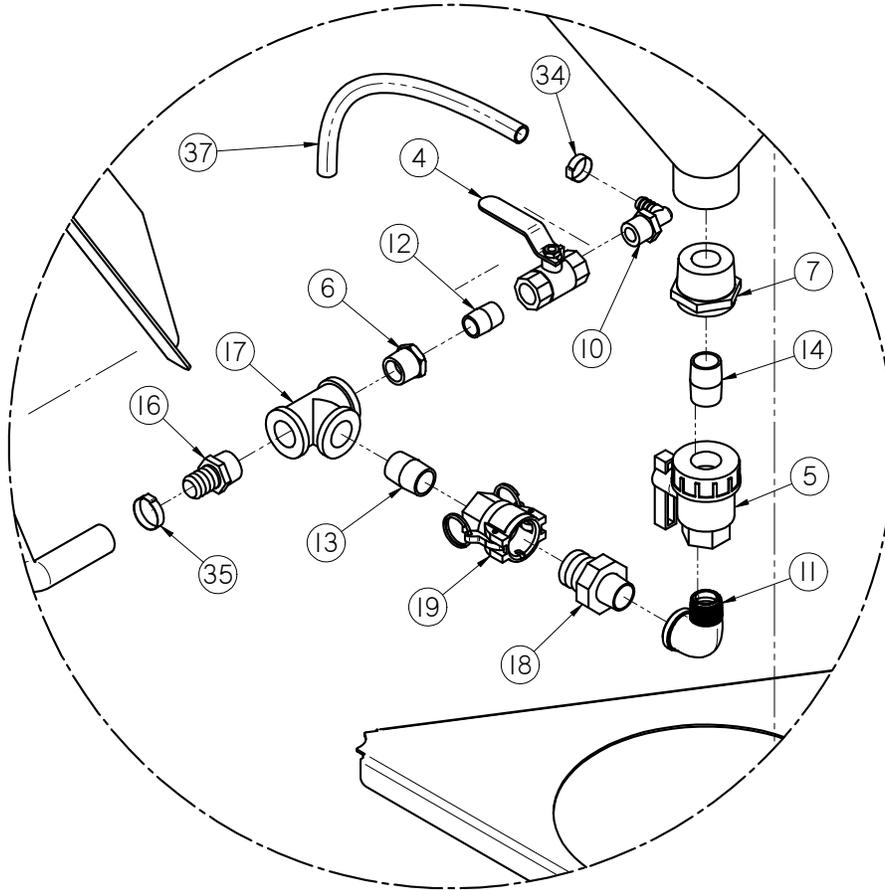

DETAIL A

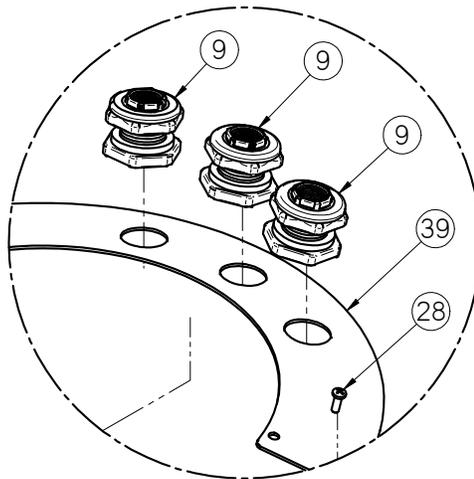

DETAIL B

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 30 Gallon Poly Tank (04-03-0161)

Item #	Part #	Description	Qty
1	01-01-0039	GBOX IL 61.8:1 56C OTP 56C INP	1
2	01-01-0080	MTR .33HP 1725RPM 56C 1PH TEFC	1
3	01-07-0015	CPLG CLPN .625 X .750 X 1.50OD SS	1
4	02-02-0006	.500-14 NPT X 2-WAY VALVE	1
5	02-02-0056	VLV BALL .750 NPT FM PLAS	1
6	02-04-0008	BUSHING .750-14 NPT, REDUCER .500-14 NPT	1
7	02-04-0034	FTTG BUSH 1.50NPT X .750NPT PPE	1
8	02-05-0028	FTTG .500 NPT DBL THD PPE BULKHEAD	1
9	02-05-0045	FTTG .750 NPT DBL THD PPE BULKHEAD	3
10	02-06-0010	FTTG 90 DEG .500HB X .500NPT ML NYL	1
11	02-06-0068	FTTG 90 DEG STRT .75NPT PPE BLK	1
12	02-07-0008	FTTG NIP .500 NPT X 1.125 TBE BLK	1
13	02-07-0025	NIPPLE 3/4" NPT CLOSE 304SS	1
14	02-07-0070	FTTG NIP .750 NPT X 1.50 TBE SS	1
15	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	1
16	02-08-0010	3/4-14 NPT TO .750 HB STRAIGHT (NYLON)	1
17	02-09-0008	TEE 3/4 NPT X 3/4 NPT X 3/4 NPT SS	1
18	02-15-0043	FTTG CPLG CAM LVR 1.5" ML X ML	1
19	02-15-0044	FTTG CPLG CAM LVR .75" FMXFM*	1
20	05-03-1133	WDMT SIDE BAFFLE 30GAL POLY	1
21	05-03-1134	WDMT 30GAL POLY LID	1
22	05-03-1135	WDMT STIR ARM 30GAL POLY	2
23	05-03-1136	WDMT LOWER STIR ARM 30GAL POLY	1
24	05-03-1298	WDMT TANKSTD 30GAL PUMPSTD	1
25	05-11-0357	ROD 30GAL DRV	1
26	06-01-0093	BOLT, .312-18 UNC 316 SS; 1 1/2" LG	4
27	06-01-0138	BOLT, FLG .315-18 UNC ZP GRADE 5; 3/4" LG	4
28	06-01-0215	SCRW MACH #14 X .750 SS PLASTITE	13
29	06-01-0262	BOLT CRG .375-16 X 4.50 FTH ZP GR5	1
30	06-02-0017	NUT FULL .313-18 SS 18-8	4
31	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	1
32	06-04-0010	WASHER, .3125 LOCK 18-8 SS	4
33	06-05-0011	WASHER, .3125 FLAT 18-8 SS	8
34	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	2
35	06-07-0030	HOSE CLAMP ONE EAR 1.004-1.126	1


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 30 Gallon Poly Tank (04-03-0161)

Item #	Part #	Description	Qty
36	07-02-0020	TNK 30GAL CONE 1.5 FPT OUTLET FD	1
37	1022B2	DRAIN HOSE PUMP STAND	1
38	1029BC	BRKT TNK CRADLE 30GAL	1
39	102A1B	BULKHEAD MNT PLT POLY TANK	1
40	102A1C	TANK MNT PLT 30GAL POLY	1
41	102C1F	HOSE TANK TO VLV	1


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 60 Gallon Poly Tank (04-03-0160)

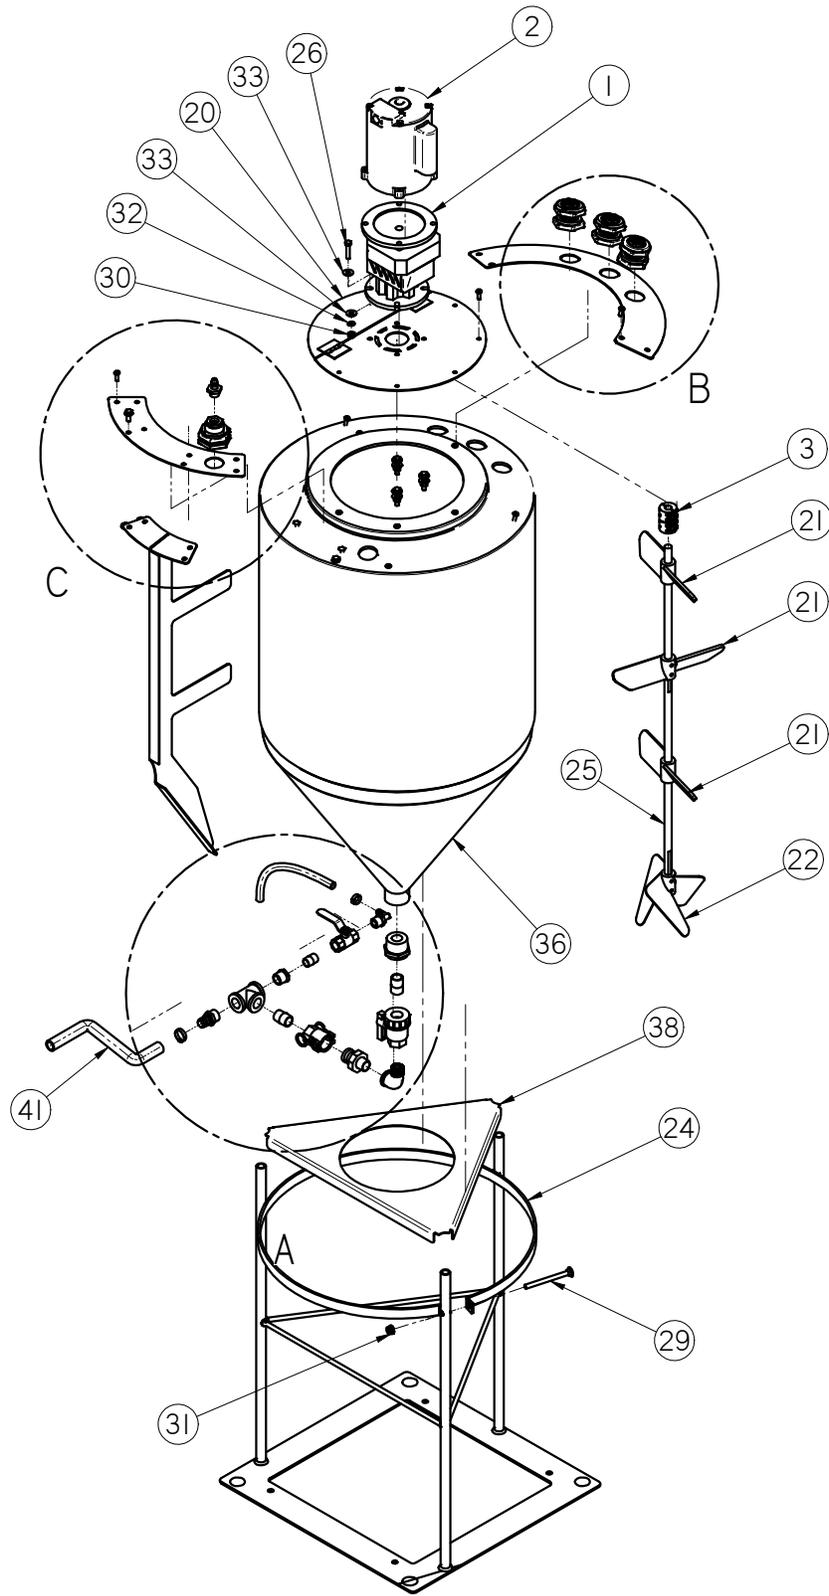


SEMI - AUTOMATED PUMP STAND


Semi - Automated Pump Stand - 60 Gallon Poly Tank (04-03-0160)

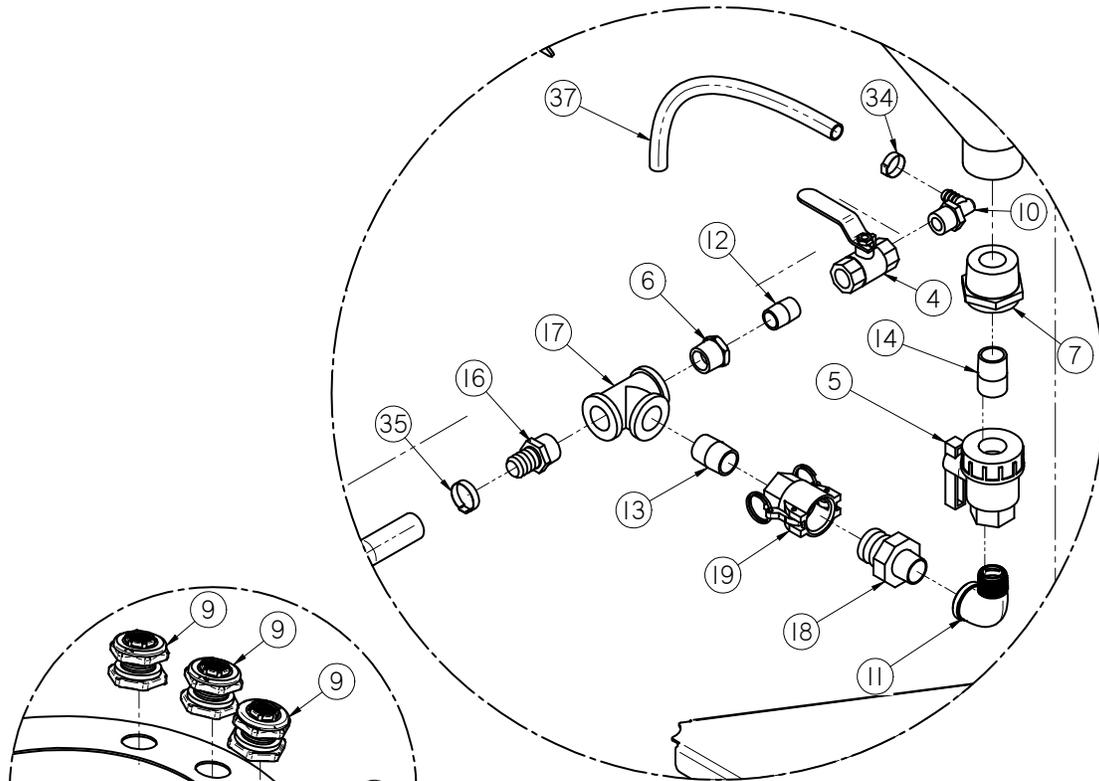

DETAIL A

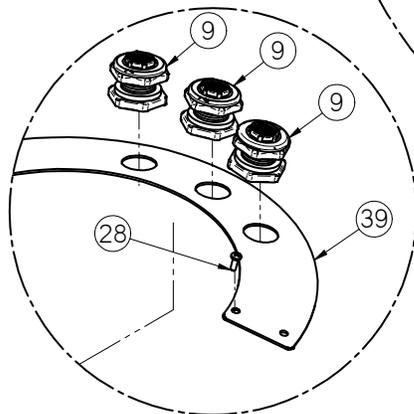

DETAIL B

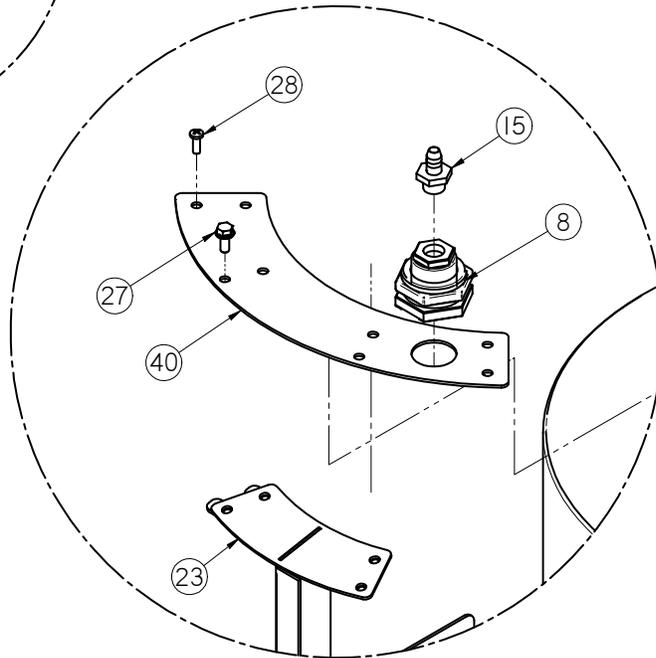

DETAIL C

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 60 Gallon Poly Tank (04-03-0160)

Item #	Part #	Description	Qty
1	01-01-0039	GBOX IL 61.8:1 56C OTP 56C INP	1
2	01-01-0080	MTR .33HP 1725RPM 56C 1PH TEFC	1
3	01-07-0015	CPLG CLPN .625 X .750 X 1.50OD SS	1
4	02-02-0006	.500-14 NPT X 2-WAY VALVE	1
5	02-02-0056	VLV BALL .750 NPT FM PLAS	1
6	02-04-0008	BUSHING .750-14 NPT, REDUCER .500-14 NPT	1
7	02-04-0034	FTTG BUSH 1.50NPT X .750NPT PPE	1
8	02-05-0028	FTTG .500 NPT DBL THD PPE BULKHEAD	1
9	02-05-0045	FTTG .750 NPT DBL THD PPE BULKHEAD	3
10	02-06-0010	FTTG 90 DEG .500HB X .500NPT ML NYL	1
11	02-06-0068	FTTG 90 DEG STRT .75NPT PPE BLK	1
12	02-07-0008	FTTG NIP .500 NPT X 1.125 TBE BLK	1
13	02-07-0025	NIPPLE 3/4" NPT CLOSE 304SS	1
14	02-07-0070	FTTG NIP .750 NPT X 1.50 TBE SS	1
15	02-08-0007	FTTG STGHT .500HB X .500NPT ML NYL	1
16	02-08-0010	3/4-14 NPT TO .750 HB STRAIGHT (NYLON)	1
17	02-09-0008	TEE 3/4 NPT X 3/4 NPT X 3/4 NPT SS	1
18	02-15-0043	FTTG CPLG CAM LVR 1.5" ML X ML	1
19	02-15-0044	FTTG CPLG CAM LVR .75" FMXFM*	1
20	05-03-1134	WDMT 30GAL POLY LID	1
21	05-03-1135	WDMT STIR ARM 30GAL POLY	3
22	05-03-1136	WDMT LOWER STIR ARM 30GAL POLY	1
23	05-03-1158	WDMT SIDE BAFFLE 60GAL POLY	1
24	05-03-1298	WDMT TANKSTD 30GAL PUMPSTD	1
25	05-11-0361	ROD 60GAL DRV	1
26	06-01-0093	BOLT, .312-18 UNC 316 SS; 1 1/2" LG	4
27	06-01-0138	BOLT, FLG .315-18 UNC ZP GRADE 5; 3/4" LG	4
28	06-01-0215	SCRW MACH #14 X .750 SS PLASTITE	13
29	06-01-0262	BOLT CRG .375-16 X 4.50 FTH ZP GR5	1
30	06-02-0017	NUT FULL .313-18 SS 18-8	4
31	06-03-0014	NUT LOCK FLG .375-16 ZP GR5	1
32	06-04-0010	WASHER, .3125 LOCK 18-8 SS	4
33	06-05-0011	WASHER, .3125 FLAT 18-8 SS	8
34	06-07-0029	HOSE CLAMP ONE EAR, .716-.827	1
35	06-07-0030	HOSE CLAMP ONE EAR 1.004-1.126	1


SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand - 60 Gallon Poly Tank (04-03-0160)

Item #	Part #	Description	Qty
36	07-02-0021	TNK 60GAL CONE 1.5 FPT OUTLET FD	1
37	1022B2	DRAIN HOSE PUMP STAND	1
38	1029BC	BRKT TNK CRADLE 30GAL	1
39	102A1B	BULKHEAD MNT PLT POLY TANK	1
40	102A1C	TANK MNT PLT 30GAL POLY	1
41	102C1E	HOSE TANK TO VLV	1

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand Assembly

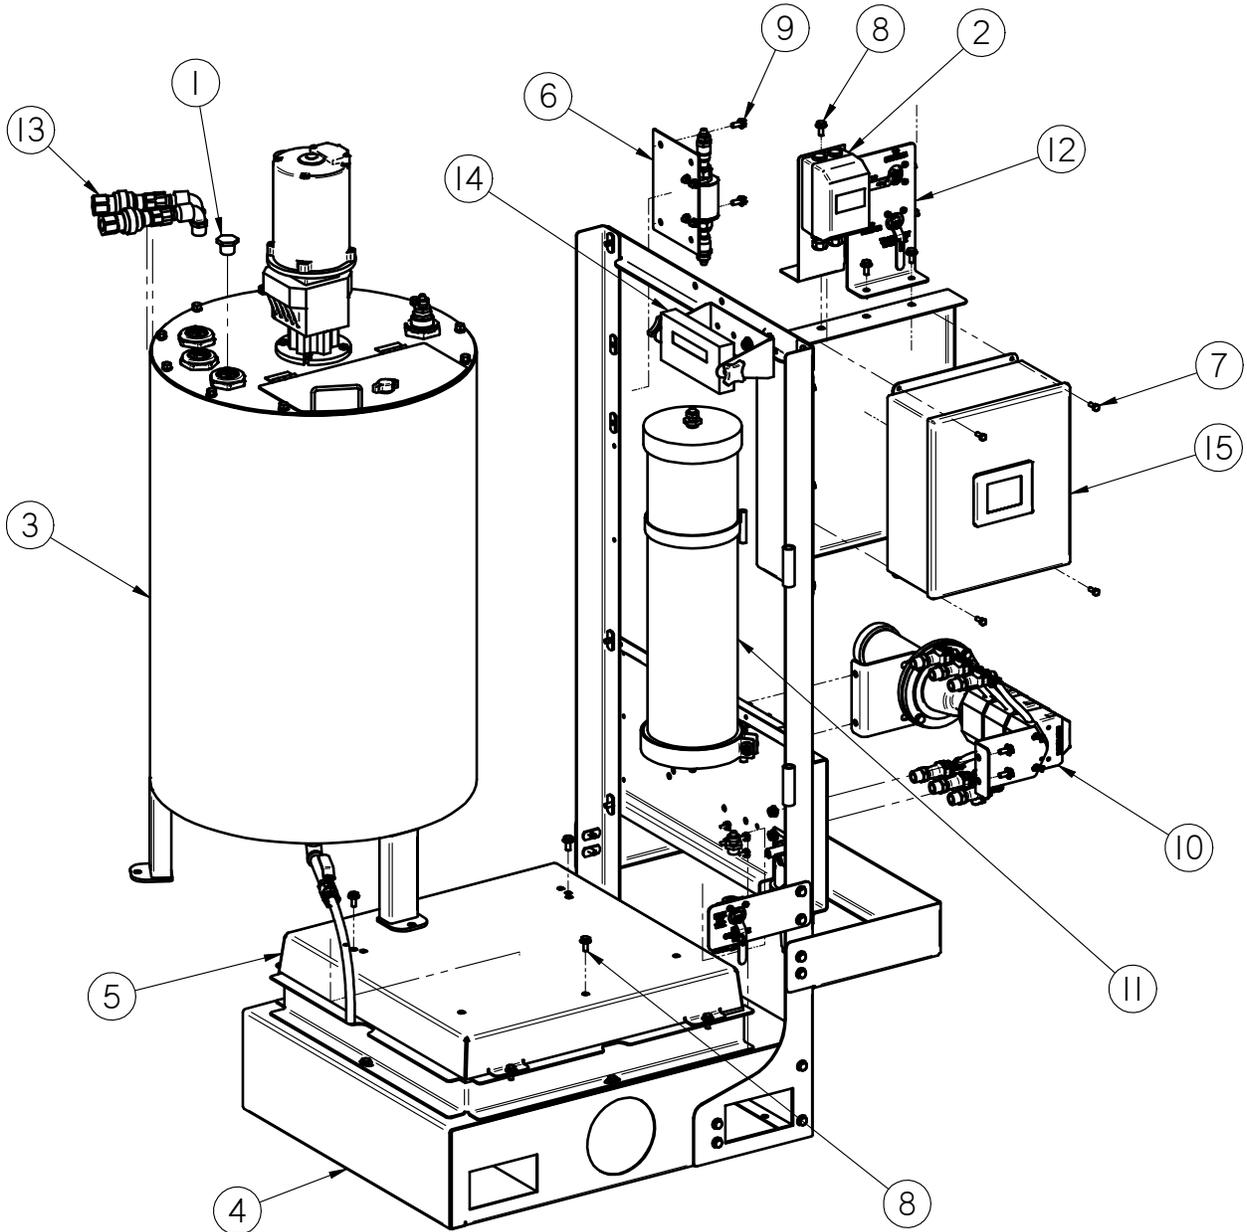

SEMI - AUTOMATED PUMP STAND

Semi - Automated Pump Stand Assembly

Item #	Part #	Description	Qty
1	02-14-0014	.750-14 NPT PLUG BP	1
2	03-13-0027	KIT SW MNL MP .33 HP MTR CHEM TNK	1
3	04-03-0158	ASSY SS 60GAL TANK PUMPSTD	1
4	05-03-1066	ASSY PUMPSTD FRAME BASE	1
5	05-03-1069	ASSY SCL PUMPSTD	1
6	05-03-1181	FLOW METER VOLUMETRIC	1
7	06-01-0006	BOLT, .250-20 X .75 UNC ZP GRADE 5	4
8	06-01-0124	BOLT, FLG .375-16 UNC ZP GRADE 5; 3/4" LG	4
9	06-01-0138	BOLT, FLG .315-18 UNC ZP GRADE 5; 3/4" LG	2
10	13-04-0103	KIT LS HEAD X3 ASSY PUMPSTD	1
11	13-04-0106	KIT CAL TUBE ASSY PUMPSTD	1
12	13-04-0109	MAN PUMPSTD CNTRLS	1
13	13-10-0017	KIT FTTG CHEM TNK .5NPT PARKER	2
14	PART OF 05-03-1069	SCALE DISPLAY	1
15	SEE TABLE 1	CONTROL PANEL	1

TABLE 1	
Part #	Description
03-12-0183A	PNL CNTL 1/4 HP MASS FM
03-12-0187A	PNL CNTL 1/10 HP MASS FM
03-12-0196A	PNL CNTL 1/4 HP VOL FM
03-12-0197B	PNL CNTL 1/10 HP VOL FM

NOTES

[Empty rectangular box for notes]

USC LIMITED WARRANTY

SECTION J

USC, LLC, (Manufacturer) warrants its seed treating equipment as follows:

1. **Limited Warranty:** Manufacturer warrants that the Products sold hereunder will be free from defects in material and workmanship for a period of 18 months from date of shipment. If the Products do not conform to this Limited Warranty during the warranty period, Buyer shall notify Manufacturer in writing of the claimed defects and demonstrate to Manufacturer satisfaction that said defects are covered by this Limited Warranty. If the defects are properly reported to Manufacturer within the warranty period, and the defects are of such type and nature as to be covered by this warranty, Manufacturer shall, at its expense, furnish replacement Products or, at Manufacturer's option, replacement parts for the defective products. Shipping and installation of the replacement Products or replacement parts shall be at the Buyer's expense.

2. **Other Limits:** THE FOREGOING IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. Manufacturer does not warrant against damages or defects arising from improper installation (where installation is by persons other than Manufacturer), against defects in products or components not manufactured by Manufacturer, or against damages resulting from such non-Manufacturer made products or components. Manufacturer passes on to the Buyer the warranty it received (if any) from the maker of such non-Manufacturer made products or components. This warranty also does not apply to Products upon which repairs and/or modifications have been effected or attempted by persons other than pursuant to written authorization by Manufacturer. Manufacturer does not warrant against casualties or damages resulting from misuse and/or abuse of product(s), acts of nature, effects of weather, including effects of weather due to outside storage, accidents, or damages incurred during transportation by common carrier.

3. **Exclusive Obligation:** THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of Manufacturer shall be to repair or replace the defective Products in the manner and for the period provided above. Manufacturer shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall Manufacturer be liable for incidental, special, or consequential damages.

4. **Other Statements:** Manufacturer's employees or representatives' oral or other written statements do not constitute warranties, shall not be relied upon by Buyer, and are not a part of the contract for sale or this limited warranty.

5. **Return Policy:** Approval is required prior to returning goods to USC, LLC. A restocking fee will apply.

6. **Entire Obligation:** This Limited Warranty states the entire obligation of Manufacturer with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.



USC, LLC

2320 124th road

Sabetha, Ks 66534

PHONE: (785) 431-7900

FAX: (785) 431-7950

EMAIL: sales-team@uscllc.com

WEB: www.uscllc.com